

CERTIFICATE OF ANALYSIS FOR


CERTIFIED REFERENCE MATERIAL

OREAS 556b

**Copper-Cobalt Ore (Kinsevere Mine, Katanga Province,
Democratic Republic of the Congo)**



Accredited for compliance with ISO 17034



COA-1785-OREAS556b-R0 BUP-70-10-01 Ver:2.0	7-Mar-2024
---	------------

TABLE OF CONTENTS

INTRODUCTION.....	10
SOURCE MATERIAL.....	10
COMMUNITION AND HOMOGENISATION PROCEDURES.....	10
PHYSICAL PROPERTIES.....	11
MINERALOGY.....	11
ANALYTICAL PROGRAM.....	12
STATISTICAL ANALYSIS.....	12
Homogeneity Evaluation.....	13
PERFORMANCE GATES.....	14
PARTICIPATING LABORATORIES.....	20
PREPARER AND SUPPLIER.....	20
METROLOGICAL TRACEABILITY.....	29
COMMUTABILITY.....	29
INTENDED USE.....	30
MINIMUM SAMPLE SIZE.....	30
PERIOD OF VALIDITY & STORAGE INSTRUCTIONS.....	30
INSTRUCTIONS FOR HANDLING & CORRECT USE.....	31
LEGAL NOTICE.....	32
DOCUMENT HISTORY.....	32
CERTIFYING OFFICER.....	32
QMS CERTIFICATION.....	32
REFERENCES.....	33
APPENDIX.....	33

LIST OF TABLES

Table 1. Certified Values, Uncertainty & Tolerance Intervals for elements by 4-Acid Digestion and Aqua Regia Digestion in OREAS 556b.....	3
Table 2. Certified Value, Uncertainty & Tolerance Intervals for other measurands in OREAS 556b.....	6
Table 3. Indicative Values for OREAS 556b.....	9
Table 4. Physical properties of OREAS 556b.....	11
Table 5. Indicative mineralogy of OREAS 556b based on semi-quantitative XRD analysis.....	11
Table 6. Performance Gates for OREAS 556b.....	14

LIST OF FIGURES

Figure 1. Co by borate fusion XRF in OREAS 556b.....	21
Figure 2. Cu by borate fusion XRF in OREAS 556b.....	22
Figure 3. Co by fusion ICP in OREAS 556b.....	23
Figure 4. Cu by fusion ICP in OREAS 556b.....	24
Figure 5. Co by 4-acid digestion in OREAS 556b.....	25
Figure 6. Cu by 4-acid digestion in OREAS 556b.....	26
Figure 7. Co by aqua regia digestion in OREAS 556b.....	27
Figure 8. Cu by aqua regia digestion in OREAS 556b.....	28

Table 1. Certified Values, Uncertainty & Tolerance Intervals for elements by 4-Acid Digestion and Aqua Regia Digestion in OREAS 556b.

Constituent	Certified Value [†]	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion					
Ag, Silver (ppm)	0.144	0.129	0.159	0.136	0.151
Al, Aluminium (wt.%)	5.67	5.54	5.80	5.56	5.77
As, Arsenic (ppm)	98	94	102	95	102
Ba, Barium (ppm)	190	183	197	183	196
Be, Beryllium (ppm)	4.52	4.37	4.67	4.40	4.64
Bi, Bismuth (ppm)	2.89	2.75	3.03	2.81	2.98
Ca, Calcium (wt.%)	0.141	0.132	0.150	0.138	0.144
Cd, Cadmium (ppm)	0.51	0.46	0.56	0.48	0.54
Ce, Cerium (ppm)	143	137	150	139	148
Co, Cobalt (wt.%)	1.99	1.95	2.04	1.96	2.03
Cr, Chromium (ppm)	89	84	94	87	91
Cs, Caesium (ppm)	1.75	1.66	1.85	1.68	1.82
Cu, Copper (wt.%)	8.64	8.48	8.80	8.53	8.75
Dy, Dysprosium (ppm)	4.54	4.10	4.97	4.36	4.71
Er, Erbium (ppm)	2.70	2.32	3.08	2.59	2.81
Eu, Europium (ppm)	0.89	0.81	0.97	0.84	0.94
Fe, Iron (wt.%)	6.71	6.56	6.85	6.60	6.81
Ga, Gallium (ppm)	28.1	26.9	29.4	27.4	28.9
Gd, Gadolinium (ppm)	4.92	4.00	5.85	4.73	5.12
Ge, Germanium (ppm)	0.23	0.18	0.28	0.21	0.25
Hf, Hafnium (ppm)	4.94	4.72	5.17	4.78	5.11
Ho, Holmium (ppm)	0.89	0.74	1.03	0.83	0.94
In, Indium (ppm)	3.56	3.38	3.75	3.46	3.67
K, Potassium (wt.%)	2.25	2.20	2.29	2.20	2.29
La, Lanthanum (ppm)	70	67	73	68	72
Li, Lithium (ppm)	52	50	53	50	53
Lu, Lutetium (ppm)	0.41	0.35	0.46	0.38	0.43
Mg, Magnesium (wt.%)	2.43	2.35	2.50	2.38	2.47
Mn, Manganese (wt.%)	0.117	0.112	0.122	0.114	0.120
Mo, Molybdenum (ppm)	18.4	17.6	19.1	17.8	18.9
Na, Sodium (wt.%)	0.049	0.044	0.054	0.046	0.052
Nb, Niobium (ppm)	14.0	12.5	15.5	13.4	14.6
Nd, Neodymium (ppm)	63	59	67	61	65
Ni, Nickel (ppm)	337	324	350	329	344
P, Phosphorus (wt.%)	0.033	0.031	0.034	0.032	0.033
Pb, Lead (ppm)	17.3	16.5	18.0	16.8	17.7

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

[†]This operationally defined measurand meets the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

Note: intervals may appear asymmetric due to rounding.

Table 1 continued.

Constituent	Certified Value [†]	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion continued					
Pr, Praseodymium (ppm)	16.5	15.2	17.8	16.0	17.1
Rb, Rubidium (ppm)	82	79	86	80	84
Re, Rhenium (ppm)	0.033	0.029	0.037	0.030	0.036
S, Sulphur (wt.%)	8.55	8.36	8.73	8.38	8.72
Sb, Antimony (ppm)	5.29	5.01	5.58	5.09	5.50
Sc, Scandium (ppm)	11.0	10.4	11.6	10.6	11.4
Se, Selenium (ppm)	11.2	10.1	12.2	10.5	11.8
Sm, Samarium (ppm)	8.58	8.01	9.15	8.29	8.87
Sn, Tin (ppm)	3.70	3.48	3.93	3.57	3.84
Sr, Strontium (ppm)	68	65	70	66	69
Ta, Tantalum (ppm)	1.04	0.93	1.15	0.99	1.09
Tb, Terbium (ppm)	0.78	0.64	0.92	0.73	0.83
Te, Tellurium (ppm)	0.089	0.063	0.116	IND	IND
Th, Thorium (ppm)	15.4	14.8	16.1	15.0	15.9
Ti, Titanium (wt.%)	0.235	0.208	0.262	0.228	0.242
Tl, Thallium (ppm)	1.06	1.00	1.12	1.02	1.09
Tm, Thulium (ppm)	0.39	0.34	0.45	0.38	0.41
U, Uranium (ppm)	8.80	8.41	9.18	8.47	9.13
V, Vanadium (ppm)	330	320	341	324	336
W, Tungsten (ppm)	2.30	2.15	2.45	2.16	2.44
Y, Yttrium (ppm)	23.5	22.6	24.4	22.8	24.1
Yb, Ytterbium (ppm)	2.72	2.47	2.97	2.62	2.82
Zn, Zinc (ppm)	38.8	37.1	40.5	37.7	39.9
Zr, Zirconium (ppm)	171	165	177	168	174
Aqua Regia Digestion					
Ag, Silver (ppm)	0.120	0.105	0.135	0.105	0.135
Al, Aluminium (wt.%)	0.869	0.791	0.947	0.827	0.912
As, Arsenic (ppm)	94	90	98	92	96
Au, Gold (ppm)	< 0.02	IND	IND	IND	IND
B, Boron (ppm)	< 10	IND	IND	IND	IND
Ba, Barium (ppm)	53	45	61	51	54
Be, Beryllium (ppm)	2.20	2.05	2.36	2.13	2.28
Bi, Bismuth (ppm)	2.82	2.67	2.97	2.75	2.89
Ca, Calcium (wt.%)	0.131	0.125	0.136	0.126	0.135
Cd, Cadmium (ppm)	0.51	0.46	0.56	0.48	0.54
Ce, Cerium (ppm)	43.6	40.3	46.9	41.8	45.3

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

[†]This operationally defined measurand meets the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value [†]	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Aqua Regia Digestion continued					
Co, Cobalt (wt.%)	1.98	1.93	2.03	1.94	2.01
Cr, Chromium (ppm)	35.0	33.5	36.5	33.9	36.1
Cs, Caesium (ppm)	0.29	0.24	0.35	0.27	0.32
Cu, Copper (wt.%)	8.55	8.39	8.71	8.44	8.67
Dy, Dysprosium (ppm)	1.02	0.84	1.19	0.95	1.08
Er, Erbium (ppm)	0.41	0.29	0.54	0.38	0.45
Eu, Europium (ppm)	0.38	0.34	0.42	0.36	0.40
Fe, Iron (wt.%)	6.65	6.49	6.80	6.54	6.75
Ga, Gallium (ppm)	9.61	8.77	10.46	9.26	9.96
Gd, Gadolinium (ppm)	1.91	1.64	2.19	1.82	2.01
Ge, Germanium (ppm)	0.13	0.09	0.16	IND	IND
Hf, Hafnium (ppm)	0.37	0.34	0.39	0.35	0.39
Hg, Mercury (ppm)	0.11	0.09	0.12	0.09	0.12
Ho, Holmium (ppm)	0.17	0.13	0.20	IND	IND
In, Indium (ppm)	2.94	2.81	3.06	2.87	3.01
K, Potassium (wt.%)	0.187	0.173	0.202	0.176	0.199
La, Lanthanum (ppm)	19.5	18.1	20.9	18.9	20.1
Li, Lithium (ppm)	31.2	28.1	34.4	30.3	32.1
Mg, Magnesium (wt.%)	1.85	1.74	1.95	1.80	1.90
Mn, Manganese (wt.%)	0.117	0.113	0.121	0.114	0.119
Mo, Molybdenum (ppm)	17.4	16.6	18.2	17.0	17.8
Na, Sodium (wt.%)	0.016	0.013	0.019	0.014	0.018
Nb, Niobium (ppm)	0.13	0.10	0.15	IND	IND
Nd, Neodymium (ppm)	23.0	18.1	27.8	21.7	24.2
Ni, Nickel (ppm)	323	310	337	316	330
P, Phosphorus (wt.%)	0.019	0.018	0.020	0.018	0.020
Pb, Lead (ppm)	14.9	14.3	15.5	14.5	15.3
Pr, Praseodymium (ppm)	5.75	4.56	6.95	5.46	6.04
Rb, Rubidium (ppm)	6.10	5.43	6.76	5.77	6.42
Re, Rhenium (ppm)	0.029	0.027	0.032	0.027	0.032
S, Sulphur (wt.%)	8.38	8.08	8.68	8.24	8.52
Sb, Antimony (ppm)	3.32	3.05	3.60	3.18	3.47
Sc, Scandium (ppm)	2.76	2.50	3.02	2.62	2.90
Se, Selenium (ppm)	10.8	9.7	11.9	10.4	11.2
Sm, Samarium (ppm)	3.50	2.90	4.11	3.29	3.71
Sn, Tin (ppm)	2.45	2.34	2.56	2.36	2.54

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

[†]This operationally defined measurand meets the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed).

Table 1 continued.

Constituent	Certified Value [†]	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Aqua Regia Digestion continued					
Sr, Strontium (ppm)	15.4	13.8	17.0	14.8	16.1
Ta, Tantalum (ppm)	< 0.01	IND	IND	IND	IND
Tb, Terbium (ppm)	0.20	0.15	0.25	0.18	0.22
Te, Tellurium (ppm)	0.075	0.058	0.092	IND	IND
Th, Thorium (ppm)	6.16	5.65	6.68	5.90	6.42
U, Uranium (ppm)	3.57	3.37	3.76	3.46	3.68
V, Vanadium (ppm)	60	56	64	58	63
W, Tungsten (ppm)	0.98	0.90	1.06	0.93	1.04
Y, Yttrium (ppm)	4.03	3.74	4.31	3.86	4.19
Yb, Ytterbium (ppm)	0.38	0.32	0.45	0.36	0.41
Zn, Zinc (ppm)	37.1	35.5	38.8	36.1	38.2
Zr, Zirconium (ppm)	11.1	10.2	11.9	10.7	11.5

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg. Note: intervals may appear asymmetric due to rounding.

[†]This operationally defined measurand meets the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

IND = indeterminate (due to limited reading resolution of the methods employed). For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 2. Certified Value, Uncertainty & Tolerance Intervals for other measurands in OREAS 556b.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate Fusion XRF					
Al ₂ O ₃ , Aluminium(III) oxide (wt.%)	10.90	10.74	11.07	10.79	11.02
BaO, Barium oxide (ppm)	242	161	323	224	260
CaO, Calcium oxide (wt.%)	0.195	0.184	0.206	0.187	0.203
Co, Cobalt (wt.%)	1.99	1.94	2.04	1.97	2.01
Cu, Copper (wt.%)	8.53	8.34	8.72	8.43	8.63
Fe ₂ O ₃ , Iron(III) oxide (wt.%)	9.68	9.53	9.83	9.59	9.77
K ₂ O, Potassium oxide (wt.%)	2.74	2.70	2.78	2.71	2.77
MgO, Magnesium oxide (wt.%)	4.11	4.05	4.16	4.06	4.15
MnO, Manganese oxide (wt.%)	0.155	0.148	0.162	0.150	0.160
Ni, Nickel (ppm)	344	308	380	320	368
P ₂ O ₅ , Phosphorus(V) oxide (wt.%)	0.080	0.074	0.085	0.077	0.083
SiO ₂ , Silicon dioxide (wt.%)	42.77	42.32	43.22	42.38	43.16
SO ₃ , Sulphur trioxide (wt.%)	21.43	20.03	22.82	21.11	21.75
Sr, Strontium (ppm)	63	27	100	IND	IND
TiO ₂ , Titanium dioxide (wt.%)	0.707	0.687	0.727	0.694	0.720
V ₂ O ₅ , Vanadium(V) oxide (ppm)	641	571	711	606	676
Zr, Zirconium (ppm)	216	194	238	IND	IND

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

IND = indeterminate (due to limited reading resolution of the methods employed).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed).

Table 2 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Thermogravimetry					
LOI ¹⁰⁰⁰ , Loss On Ignition @1000°C (wt.%)	14.41	14.20	14.62	14.32	14.50
Infrared Combustion					
C, Carbon (wt.%)	4.58	4.48	4.68	4.54	4.62
S, Sulphur (wt.%)	8.78	8.67	8.90	8.71	8.86
Sulphuric Acid 5% Leach					
Co, Cobalt (wt.%)	0.685	0.639	0.732	0.664	0.706
Cu, Copper (wt.%)	1.32	1.25	1.38	1.30	1.34
Peroxide Fusion ICP					
Al, Aluminium (wt.%)	5.71	5.58	5.84	5.58	5.84
As, Arsenic (ppm)	101	95	108	98	104
B, Boron (ppm)	199	166	233	186	213
Ba, Barium (ppm)	196	185	207	187	205
Be, Beryllium (ppm)	5.06	4.62	5.50	IND	IND
Bi, Bismuth (ppm)	3.08	2.87	3.28	2.81	3.34
Ca, Calcium (wt.%)	0.149	0.121	0.176	0.134	0.163
Ce, Cerium (ppm)	156	144	168	143	169
Co, Cobalt (wt.%)	1.99	1.91	2.07	1.94	2.04
Cr, Chromium (ppm)	113	100	125	106	119
Cs, Caesium (ppm)	1.86	1.66	2.06	1.68	2.04
Cu, Copper (wt.%)	8.63	8.41	8.85	8.50	8.76
Dy, Dysprosium (ppm)	6.28	5.75	6.81	5.93	6.62
Er, Erbium (ppm)	3.47	3.22	3.71	3.30	3.63
Eu, Europium (ppm)	0.88	0.71	1.05	0.82	0.93
Fe, Iron (wt.%)	6.73	6.56	6.90	6.60	6.86
Ga, Gallium (ppm)	28.7	26.5	30.8	26.8	30.5
Gd, Gadolinium (ppm)	6.90	6.48	7.32	6.49	7.31
Ge, Germanium (ppm)	2.80	2.39	3.22	2.51	3.10
Ho, Holmium (ppm)	1.22	1.11	1.33	1.15	1.28
In, Indium (ppm)	3.52	3.25	3.78	3.32	3.71
K, Potassium (wt.%)	2.27	2.20	2.34	2.20	2.34
La, Lanthanum (ppm)	75	71	79	72	78
Li, Lithium (ppm)	51	45	57	50	52
Lu, Lutetium (ppm)	0.53	0.41	0.65	0.49	0.57
Mg, Magnesium (wt.%)	2.49	2.42	2.56	2.44	2.54
Mn, Manganese (wt.%)	0.121	0.114	0.128	0.115	0.126
Mo, Molybdenum (ppm)	18.7	17.0	20.5	17.4	20.1
Nb, Niobium (ppm)	22.5	19.7	25.2	20.8	24.2

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed).

Table 2 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Peroxide Fusion ICP continued					
Nd, Neodymium (ppm)	62	55	69	59	65
Ni, Nickel (ppm)	343	326	360	332	353
P, Phosphorus (wt.%)	0.035	0.025	0.044	IND	IND
Pb, Lead (ppm)	< 100	IND	IND	IND	IND
Pr, Praseodymium (ppm)	18.3	16.8	19.7	17.5	19.0
Rb, Rubidium (ppm)	82	78	86	79	85
S, Sulphur (wt.%)	8.75	8.49	9.01	8.56	8.94
Sb, Antimony (ppm)	5.77	5.10	6.45	5.08	6.47
Sc, Scandium (ppm)	9.56	7.46	11.66	IND	IND
Si, Silicon (wt.%)	20.48	19.91	21.04	20.14	20.82
Sm, Samarium (ppm)	8.88	7.76	9.99	8.29	9.46
Sr, Strontium (ppm)	73	69	77	71	75
Ta, Tantalum (ppm)	1.84	1.53	2.16	IND	IND
Tb, Terbium (ppm)	1.05	0.96	1.15	0.98	1.13
Th, Thorium (ppm)	15.5	14.5	16.5	14.9	16.1
Ti, Titanium (wt.%)	0.414	0.403	0.425	0.402	0.426
Tl, Thallium (ppm)	1.06	0.94	1.18	IND	IND
Tm, Thulium (ppm)	0.52	0.48	0.57	0.48	0.56
U, Uranium (ppm)	8.85	8.05	9.65	8.46	9.24
V, Vanadium (ppm)	353	338	368	343	363
W, Tungsten (ppm)	2.96	2.13	3.80	IND	IND
Y, Yttrium (ppm)	32.6	30.8	34.4	31.2	34.0
Yb, Ytterbium (ppm)	3.19	2.86	3.52	2.95	3.43
Zn, Zinc (ppm)	41.4	35.8	46.9	38.4	44.3

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 3. Indicative Values for OREAS 556b.

Constituent	Unit	Value	Constituent	Unit	Value	Constituent	Unit	Value
Borate Fusion XRF continued								
Ag	ppm	0.021	HfO ₂	ppm	429	Sc	ppm	11.9
As	ppm	86	Hg	ppm	< 100	Se	ppm	2.33
Be	ppm	3.00	Ho	ppm	1.22	Sm	ppm	8.79
Bi	ppm	< 100	In	ppm	3.80	Sn	ppm	106
Cd	ppm	< 100	La	ppm	77	Ta	ppm	1.25
Ce	ppm	153	Lu	ppm	0.51	Tb	ppm	1.02
Cl	ppm	249	Mo	ppm	< 50	Te	ppm	11.1
Cr ₂ O ₃	ppm	185	Na ₂ O	wt.%	0.107	Th	ppm	15.6
Cs	ppm	1.98	Nb	ppm	56	Tl	ppm	0.85
Dy	ppm	5.97	Nd	ppm	60	Tm	ppm	0.52
Er	ppm	3.41	Pb	ppm	81	U	ppm	8.95
Eu	ppm	0.83	Pr	ppm	16.5	W	ppm	6.26
Ga	ppm	28.8	Rb	ppm	99	Y	ppm	33.1
Gd	ppm	6.48	Re	ppm	22.6	Yb	ppm	3.30
Ge	ppm	< 100	Sb	ppm	< 50	Zn	ppm	44.4
Peroxide Fusion ICP								
Ag	ppm	0.453	Na	wt.%	0.045	Te	ppm	< 2
Cd	ppm	< 10	Re	ppm	0.059	Zr	ppm	209
Hf	ppm	6.41	Se	ppm	16.7			
Hg	ppm	0.083	Sn	ppm	3.64			
4-Acid Digestion								
Hg	ppm	0.13	Pt	ppb	11.2			
Aqua Regia Digestion								
Ir	ppm	< 0.003	Pt	ppb	< 5	Tm	ppm	0.056
Lu	ppm	0.060	Ti	wt.%	0.003			
Pd	ppb	< 10	Tl	ppm	0.37			
3-Acid Digestion (no HF)								
Ag	ppm	0.390	Gd	ppm	5.47	S	wt.%	7.88
Al ₂ O ₃	wt.%	10.50	Hf	ppm	5.50	Sc	ppm	11.4
Ba	ppm	180	Ho	ppm	0.86	Sm	ppm	8.18
Be	ppm	5.45	K ₂ O	wt.%	2.68	Sn	ppm	3.62
Bi	ppm	3.47	La	ppm	77	Sr	ppm	67
CaO	wt.%	0.177	Li	ppm	53	Ta	ppm	0.31
Cd	ppm	0.65	MgO	wt.%	4.03	Tb	ppm	0.68
Ce	ppm	137	MnO	wt.%	0.146	Th	ppm	17.3
Co	wt.%	2.08	Mo	ppm	20.8	TiO ₂	wt.%	0.669
Cr	ppm	98	Na ₂ O	wt.%	0.067	U	ppm	9.50
Cs	ppm	1.78	Nb	ppm	20.3	V	ppm	332
Cu	wt.%	8.94	Nd	ppm	64	W	ppm	2.95
Dy	ppm	4.62	Ni	ppm	383	Y	ppm	25.9
Er	ppm	2.75	P ₂ O ₅	wt.%	< 0.002	Yb	ppm	2.74
Eu	ppm	0.94	Pb	ppm	19.7	Zn	ppm	76
Fe ₂ O ₃	wt.%	9.34	Pr	ppm	17.2	Zr	ppm	179
Ga	ppm	27.6	Rb	ppm	82			

SI unit equivalents: ppb (parts per billion; 1×10^{-9}) \equiv $\mu\text{g}/\text{kg}$; ppm (parts per million; 1×10^{-6}) \equiv mg/kg ; wt.% (weight per cent) \equiv % (mass fraction).

Note: the number of significant figures reported is not a reflection of the level of certainty of stated values. They are instead an artefact of ORE's in-house CRM-specific LIMS.

INTRODUCTION

OREAS reference materials are intended to provide a low-cost method of evaluating and improving the quality of analysis of geological samples. To the geologist they provide a means of implementing quality control in analytical data sets generated in exploration from the grass roots level through to prospect evaluation, and in grade control at mining operations. To the analyst they provide an effective means of calibrating analytical equipment, assessing new techniques and routinely monitoring in-house procedures. OREAS reference materials enable users to successfully achieve process control of these tasks because the observed variance from repeated analysis has its origin almost exclusively in the analytical process rather than the reference material itself. In evaluating laboratory performance with this CRM, the section headed 'Instructions for correct use' should be read carefully.

Table 1 and 2 provides the certified values and their associated 95% expanded uncertainty and tolerance intervals, Table 3 shows indicative values, Table 4 provides some indicative physical properties, Table 5 provides indicative mineralogy based on semi-quantitative XRD analysis and Table 6 presents the performance gate intervals for all certified values. Tabulated results of all elements together with uncorrected means, medians, standard deviations, relative standard deviations and per cent deviation of lab means from the corrected mean of means (PDM³) are presented in the detailed certification data for this CRM (**OREAS 556b-DataPack.1.0.240216_190018.xlsx**).

Results are also presented in scatter plots for Co and Cu by multiple operationally defined methods including borate fusion with XRF finish, peroxide fusion with ICP-OES/MS finish, 4-acid digestion with ICP-OES/MS finish (and/or AAS finish) and aqua regia digestion with ICP-OES/MS finish (and/or AAS finish) in Figures 1 to 8 respectively, together with $\pm 3SD$ (magenta) and $\pm 5\%$ (yellow) control lines and certified value (green line). Accepted individual results are coloured blue and individual and dataset outliers are identified in red and violet, respectively.

SOURCE MATERIAL

OREAS 556b was prepared from copper-cobalt sulphide ore samples sourced from MMG's Kinsevere Mine blended with barren black slate and a minor addition of cobalt concentrate. The Kinsevere Mine is located in the Haut-Katanga province about 30 km from Lubumbashi in the south-east of the Democratic Republic of the Congo (DRC). The hypogene mineralisation at Kinsevere occurs as stratabound, veins and breccias consisting of mainly chalcopyrite, carrollite, bornite and occasionally pyrite and chalcocite, hosted within the Mine series carbonaceous shales, siltstones, and dolomites of the Roan Group belonging to the Katangan Supergroup stratigraphy.

COMMINUTION AND HOMOGENISATION PROCEDURES

The material constituting OREAS 556b was prepared in the following manner:

- Drying of ore and barren materials to constant mass at 105°C;
- Drying of cobalt concentrate to constant mass at 95°C;
- Crushing and milling of the ore materials to 100% minus 30 microns;
- Crushing and milling of the barren materials to >98% minus 75 microns;

- Deagglomeration of cobalt concentrate and screening at 150 microns;
- Check analysis of ores and concentrate for contained Co and Cu concentrations;
- Blending ores, Co concentrate and barren materials in appropriate proportions to achieve the desired grades;
- Homogenisation using OREAS' novel processing technologies;
- Packaging in 10g units sealed under nitrogen in laminated foil pouches.

PHYSICAL PROPERTIES

OREAS 556b was tested at ORE Research & Exploration Pty Ltd's onsite facility for various physical properties. Table 4 presents these findings that should be used for informational purposes only.

Table 4. Physical properties of OREAS 556b.

Bulk Density (kg/m ³)	Moisture (wt.%)	Munsell Notation [‡]	Munsell Color [‡]
773	0.33	N2	GrayishBlack

[‡]The Munsell Rock Color Chart helps geologists and archeologists communicate with colour more effectively by cross-referencing ISCC-NBS colour names with unique Munsell alpha-numeric colour notations for rock colour samples.

MINERALOGY

The semi-quantitative XRD results shown in Table 5 below have been normalised to 100 % and represent the relative proportion of crystalline material. Totals greater or less than 100 % are due to rounding errors. Some amorphous material might be present. A trace amount of plagioclase appears to be present. The quantification of the kandite group is performed on a largely overlapped pattern and carries high than usual uncertainty. A trace amount of arsenopyrite and malachite may also be present.

Table 5. Indicative mineralogy of OREAS 556b based on semi-quantitative XRD analysis.

Mineral / Mineral Group	% (mass ratio)
Chlorite	4
Kandite group	2
Annite - biotite - phlogopite	2
Muscovite	14
K-feldspar and/or rutile	0
Tourmaline	< 1
Quartz	36
Dolomite - ankerite	< 1
Pyrite	< 1
Chalcopyrite	20
Linnaeite group	6
Magnetite and/or antlerite	1
Goethite	1
Malachite	0
Magnesite	11
Rutile	1

ANALYTICAL PROGRAM

Thirty analytical laboratories participated in the program to characterise the elements reported in Tables 1 and 2. The following elements and methods were undertaken:

- Lithium borate fusion whole rock analysis package by X-ray fluorescence (up to 20 laboratories depending on the element; except for one laboratory that used pressed powder pellet with XRF);
- Loss on Ignition (LOI) at 1000° C (14 laboratories used a thermogravimetric analyser, 6 laboratories included LOI with their fusion package and 4 laboratories used a conventional muffle furnace);
- Infrared combustion furnace/CS analyser to determine C (25 laboratories) and S (26 laboratories);
- Co (9 laboratories) and Cu (19 laboratories) by *5% sulphuric acid leach with ICP-OES or AAS finish;
- Full ICP-OES and ICP-MS elemental suites by sodium peroxide fusion (up to 22 laboratories depending on the element);
- Full ICP-OES and ICP-MS elemental suites by 4-acid (HCl-HNO₃-HF-HClO₄) digestion (up to 27 laboratories depending on the element);
- Full ICP-OES and ICP-MS elemental suites by aqua regia digestion (up to 27 laboratories depending on the element).

*See 'Appendix' for specified methodology.

For the round robin program, ten 800g test units were taken at predetermined intervals immediately following homogenisation and are considered representative of the entire prepared batch. The six samples received by each laboratory were obtained by taking two 30g scoop splits from each of three separate 800g test units. This format enabled a nested ANOVA treatment of the results to evaluate homogeneity, i.e., to ascertain whether between-unit variance is greater than within-unit variance (see 'Homogeneity Evaluation' section below).

STATISTICAL ANALYSIS

Certified Values and their uncertainty intervals (Tables 1 and 2) have been determined for each analyte following removal of individual, laboratory dataset (batch) and 3SD outliers (single iteration).

For individual outliers within a laboratory batch the z-score test is used in combination with a second method that determines the per cent deviation of the individual value from the batch median. Outliers in general are selected on the basis of z-scores > 2.5 and with per cent deviations (i) > 3 and (ii) more than three times the average absolute per cent deviation for the batch. Each laboratory data set mean is tested for outlying status based on z-score discrimination and rejected if > 2.5. After individual and laboratory data set (batch) outliers have been eliminated a non-iterative 3 standard deviation filter is applied, with those values lying outside this window also relegated to outlying status. However, while statistics are taken into account, the exercise of a statistician's prerogative plays a significant role in identifying outliers.

95% Expanded Uncertainty provides a 95% probability that the true value of the analyte under consideration lies between the upper and lower limits and is calculated according to the method outlined in ISO 98-3:2008 [5]. All known or suspected sources of bias have been investigated or taken into account.

Indicative (uncertified) values (Table 3) are present where the number of laboratories reporting a particular analyte is insufficient (< 5) to support certification or where interlaboratory consensus is poor.

Standard Deviation intervals (see Table 5) provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this CRM in a QA/QC program. They take into account errors attributable to measurement uncertainty and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. The Standard Deviation values include all sources of measurement uncertainty: between-lab variance, within-run variance (precision errors) and CRM variability.

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program (see 'Intended Use' section for more detail).

The SD for each analyte's certified value is calculated from the same filtered data set used to determine the certified value, i.e., after removal of all individual, lab dataset (batch) and 3SD outliers (single iteration). These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e., the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM. ***The standard deviation is then calculated for each analyte from the pooled accepted analyses generated from the certification program.***

Homogeneity Evaluation

The tolerance limits (ISO 16269:2014) shown in Tables 1 and 2 were determined using an analysis of precision errors method and are considered a conservative estimate of true homogeneity. The meaning of tolerance limits may be illustrated for copper by fusion with XRF, where 99% of the time ($1-\alpha=0.99$) at least 95% of subsamples ($p=0.95$) will have concentrations lying between 8.43 and 8.63 wt.%. Put more precisely, this means that if the same number of subsamples were taken and analysed in the same manner repeatedly, 99% of the tolerance intervals so constructed would cover at least 95% of the total population, and 1% of the tolerance intervals would cover less than 95% of the total population (ISO Guide 35). ***Please note that tolerance limits pertain to the homogeneity of the CRM only and should not be used as control limits for laboratory performance.***

The homogeneity of OREAS 556b has also been evaluated in an ANOVA study for all certified analytes present in concentrations well above detection levels (i.e. >20 x Lower Limit of Detection) for the various methods undertaken. This study tests the null hypothesis that no statistically significant difference exists between the between-unit variance and the within-unit variance (i.e. p -values <0.05 indicate rejection of the null hypothesis). Of the 194 certified values, no failures were observed indicating no evidence to reject the null hypothesis.

Based on the statistical analysis of ANOVA and the results of the interlaboratory certification program, it can be concluded that OREAS 556b is fit-for-purpose as a certified reference material (see 'Intended Use' below).

PERFORMANCE GATES

The standard deviations (SD's) intervals reported in Table 6 provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this CRM in a QA/QC program. They take into account errors attributable to measurement uncertainty and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. The Standard Deviation values include all sources of measurement uncertainty: between-lab variance, within-run variance (precision errors) and CRM variability.

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program (see 'Instructions for handling and correct use' section for more detail). The SD for each analyte's certified value is calculated from the same filtered data set used to determine the certified value, i.e., after removal of all individual, lab dataset (batch) and 3SD outliers (single iteration). These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e., the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM.

The standard deviation is then calculated for each analyte from the pooled accepted analyses generated from the certification program.

Table 6 below shows intervals calculated for two and three standard deviations. As a guide these intervals may be regarded as warning or rejection for multiple 2SD outliers, or rejection for individual 3SD outliers in QC monitoring, although their precise application should be at the discretion of the QC manager concerned (also see 'Intended Use' section below). Westgard Rules extend the basics of single-rule QC monitoring using multi-rules (for more information visit www.westgard.com/mltirule.htm). A second method utilises a 5% window calculated directly from the certified value. Standard deviation is also shown in relative percent for one, two and three relative standard deviations (1RSD, 2RSD and 3RSD) to facilitate an appreciation of the magnitude of these numbers and a comparison with the 5% window. Caution should be exercised when concentration levels approach lower limits of detection of the analytical methods employed as performance gates calculated from standard deviations tend to be excessively wide whereas those determined by the 5% method are too narrow. One approach used at commercial laboratories is to set the acceptance criteria at twice the detection level (DL) $\pm 10\%$.

i.e., Certified Value $\pm 10\% \pm 2DL$ [1].

Table 6. Performance Gates for OREAS 556b.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate Fusion XRF											
Al ₂ O ₃ , wt. %	10.90	0.243	10.42	11.39	10.17	11.63	2.23%	4.46%	6.69%	10.36	11.45
BaO, ppm	242	60	121	363	61	423	24.95%	49.90%	74.86%	230	254
CaO, wt. %	0.195	0.008	0.179	0.211	0.171	0.219	4.12%	8.24%	12.35%	0.186	0.205
Co, wt. %	1.99	0.056	1.88	2.10	1.82	2.16	2.80%	5.61%	8.41%	1.89	2.09
Cu, wt. %	8.53	0.257	8.01	9.04	7.76	9.30	3.01%	6.02%	9.04%	8.10	8.95
Fe ₂ O ₃ , wt. %	9.68	0.211	9.26	10.10	9.05	10.31	2.18%	4.36%	6.54%	9.20	10.16
K ₂ O, wt. %	2.74	0.070	2.60	2.88	2.53	2.95	2.55%	5.10%	7.64%	2.60	2.88
MgO, wt. %	4.11	0.080	3.95	4.27	3.87	4.35	1.95%	3.91%	5.86%	3.90	4.31
MnO, wt. %	0.155	0.006	0.143	0.167	0.137	0.173	3.85%	7.71%	11.56%	0.147	0.162
Ni, ppm	344	45	254	434	209	479	13.08%	26.16%	39.23%	327	361
P ₂ O ₅ , wt. %	0.080	0.007	0.066	0.094	0.059	0.101	8.70%	17.40%	26.10%	0.076	0.084
SiO ₂ , wt. %	42.77	0.708	41.35	44.19	40.65	44.90	1.66%	3.31%	4.97%	40.63	44.91
SO ₃ , wt. %	21.43	1.457	18.51	24.34	17.05	25.80	6.80%	13.60%	20.41%	20.36	22.50
Sr, ppm	63	16	32	95	16	110	24.78%	49.57%	74.35%	60	66
TiO ₂ , wt. %	0.707	0.032	0.642	0.772	0.610	0.804	4.58%	9.16%	13.74%	0.672	0.742
V ₂ O ₅ , ppm	641	80	480	801	400	882	12.52%	25.05%	37.57%	609	673
Zr, ppm	216	30	155	277	125	307	14.08%	28.15%	42.23%	205	227
Thermogravimetry											
LOI ¹⁰⁰⁰ , wt. %	14.41	0.332	13.75	15.07	13.41	15.40	2.30%	4.60%	6.91%	13.69	15.13
Infrared Combustion											
C, wt. %	4.58	0.193	4.19	4.97	4.00	5.16	4.21%	8.43%	12.64%	4.35	4.81
S, wt. %	8.78	0.138	8.51	9.06	8.37	9.20	1.57%	3.14%	4.71%	8.35	9.22
Sulphuric Acid 5% Leach											
Co, wt. %	0.685	0.045	0.595	0.776	0.550	0.821	6.60%	13.20%	19.80%	0.651	0.720
Cu, wt. %	1.32	0.093	1.13	1.50	1.04	1.60	7.09%	14.18%	21.27%	1.25	1.38
Peroxide Fusion ICP											
Al, wt. %	5.71	0.164	5.38	6.04	5.22	6.20	2.87%	5.75%	8.62%	5.42	5.99
As, ppm	101	7	87	116	80	123	7.12%	14.24%	21.36%	96	106
B, ppm	199	37	125	274	88	311	18.65%	37.29%	55.94%	189	209
Ba, ppm	196	9	178	213	169	222	4.50%	9.00%	13.51%	186	205
Be, ppm	5.06	0.413	4.24	5.89	3.82	6.30	8.16%	16.31%	24.47%	4.81	5.31
Bi, ppm	3.08	0.131	2.81	3.34	2.68	3.47	4.25%	8.50%	12.75%	2.92	3.23
Ca, wt. %	0.149	0.028	0.093	0.205	0.065	0.232	18.79%	37.59%	56.38%	0.141	0.156
Ce, ppm	156	6	144	168	139	173	3.71%	7.42%	11.13%	148	164
Co, wt. %	1.99	0.079	1.83	2.15	1.76	2.23	3.95%	7.90%	11.84%	1.89	2.09
Cr, ppm	113	18	77	148	59	166	15.87%	31.75%	47.62%	107	118
Cs, ppm	1.86	0.118	1.62	2.09	1.51	2.21	6.33%	12.66%	18.98%	1.77	1.95
Cu, wt. %	8.63	0.271	8.09	9.17	7.82	9.44	3.13%	6.27%	9.40%	8.20	9.06
Dy, ppm	6.28	0.290	5.70	6.86	5.41	7.15	4.62%	9.23%	13.85%	5.96	6.59
Er, ppm	3.47	0.226	3.02	3.92	2.79	4.14	6.51%	13.01%	19.52%	3.29	3.64
Eu, ppm	0.88	0.13	0.62	1.14	0.49	1.27	14.74%	29.49%	44.23%	0.83	0.92
Fe, wt. %	6.73	0.211	6.31	7.15	6.10	7.36	3.13%	6.26%	9.39%	6.39	7.07
Ga, ppm	28.7	1.90	24.9	32.5	23.0	34.4	6.63%	13.26%	19.89%	27.2	30.1
Gd, ppm	6.90	0.327	6.25	7.55	5.92	7.88	4.74%	9.48%	14.22%	6.55	7.24

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Peroxide Fusion ICP continued											
Ge, ppm	2.80	0.36	2.08	3.53	1.71	3.90	12.98%	25.96%	38.95%	2.66	2.94
Ho, ppm	1.22	0.093	1.03	1.40	0.94	1.49	7.62%	15.24%	22.86%	1.16	1.28
In, ppm	3.52	0.215	3.09	3.95	2.87	4.16	6.11%	12.22%	18.32%	3.34	3.69
K, wt. %	2.27	0.085	2.10	2.44	2.02	2.52	3.73%	7.47%	11.20%	2.16	2.38
La, ppm	75	3.9	67	83	64	87	5.17%	10.34%	15.51%	71	79
Li, ppm	51	5	41	61	36	66	10.05%	20.10%	30.15%	48	54
Lu, ppm	0.53	0.09	0.35	0.71	0.26	0.80	16.81%	33.61%	50.42%	0.51	0.56
Mg, wt. %	2.49	0.087	2.31	2.66	2.23	2.75	3.51%	7.01%	10.52%	2.36	2.61
Mn, wt. %	0.121	0.007	0.106	0.135	0.099	0.143	6.06%	12.12%	18.18%	0.115	0.127
Mo, ppm	18.7	2.0	14.8	22.7	12.8	24.7	10.54%	21.07%	31.61%	17.8	19.7
Nb, ppm	22.5	1.74	19.0	25.9	17.3	27.7	7.73%	15.46%	23.20%	21.3	23.6
Nd, ppm	62	3.3	55	68	52	72	5.35%	10.70%	16.05%	59	65
Ni, ppm	343	26	292	394	266	419	7.45%	14.91%	22.36%	325	360
P, wt. %	0.035	0.007	0.022	0.048	0.015	0.054	18.76%	37.52%	56.29%	0.033	0.036
Pb, ppm	< 100	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Pr, ppm	18.3	0.83	16.6	19.9	15.8	20.8	4.56%	9.12%	13.68%	17.4	19.2
Rb, ppm	82	2.9	76	88	73	91	3.56%	7.12%	10.68%	78	86
S, wt. %	8.75	0.277	8.20	9.31	7.92	9.58	3.16%	6.32%	9.48%	8.31	9.19
Sb, ppm	5.77	0.450	4.87	6.67	4.42	7.12	7.79%	15.58%	23.36%	5.48	6.06
Sc, ppm	9.56	1.81	5.94	13.18	4.13	14.99	18.92%	37.84%	56.77%	9.08	10.04
Si, wt. %	20.48	0.479	19.52	21.43	19.04	21.91	2.34%	4.68%	7.01%	19.45	21.50
Sm, ppm	8.88	0.97	6.93	10.82	5.95	11.80	10.98%	21.96%	32.94%	8.43	9.32
Sr, ppm	73	6.9	60	87	53	94	9.36%	18.73%	28.09%	70	77
Ta, ppm	1.84	0.27	1.30	2.38	1.03	2.65	14.65%	29.30%	43.96%	1.75	1.93
Tb, ppm	1.05	0.062	0.93	1.18	0.87	1.24	5.84%	11.67%	17.51%	1.00	1.11
Th, ppm	15.5	0.87	13.8	17.3	12.9	18.1	5.63%	11.26%	16.89%	14.7	16.3
Ti, wt. %	0.414	0.014	0.386	0.442	0.372	0.456	3.41%	6.82%	10.24%	0.393	0.435
Tl, ppm	1.06	0.096	0.87	1.25	0.77	1.35	9.04%	18.08%	27.12%	1.01	1.11
Tm, ppm	0.52	0.040	0.44	0.60	0.40	0.64	7.57%	15.14%	22.72%	0.50	0.55
U, ppm	8.85	0.90	7.06	10.64	6.16	11.54	10.13%	20.27%	30.40%	8.41	9.29
V, ppm	353	19	314	392	294	411	5.53%	11.06%	16.58%	335	370
W, ppm	2.96	0.48	2.01	3.92	1.53	4.40	16.11%	32.23%	48.34%	2.82	3.11
Y, ppm	32.6	2.60	27.4	37.8	24.8	40.4	7.96%	15.92%	23.88%	31.0	34.2
Yb, ppm	3.19	0.271	2.65	3.73	2.38	4.00	8.49%	16.98%	25.47%	3.03	3.35
Zn, ppm	41.4	3.54	34.3	48.4	30.7	52.0	8.57%	17.14%	25.71%	39.3	43.4
4-Acid Digestion											
Ag, ppm	0.144	0.013	0.118	0.170	0.105	0.183	9.00%	18.00%	26.99%	0.137	0.151
Al, wt. %	5.67	0.152	5.36	5.97	5.21	6.13	2.69%	5.38%	8.07%	5.38	5.95
As, ppm	98	4.6	89	108	84	112	4.73%	9.47%	14.20%	93	103
Ba, ppm	190	10	170	210	160	219	5.22%	10.45%	15.67%	180	199
Be, ppm	4.52	0.210	4.10	4.94	3.89	5.15	4.64%	9.29%	13.93%	4.29	4.74
Bi, ppm	2.89	0.178	2.54	3.25	2.36	3.43	6.13%	12.27%	18.40%	2.75	3.04
Ca, wt. %	0.141	0.009	0.122	0.160	0.113	0.169	6.70%	13.41%	20.11%	0.134	0.148
Cd, ppm	0.51	0.06	0.39	0.63	0.33	0.69	11.50%	23.00%	34.50%	0.48	0.54

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion continued											
Ce, ppm	143	7	129	157	122	164	4.88%	9.77%	14.65%	136	151
Co, wt. %	1.99	0.061	1.87	2.11	1.81	2.17	3.04%	6.07%	9.11%	1.89	2.09
Cr, ppm	89	7.8	73	105	66	112	8.78%	17.57%	26.35%	85	93
Cs, ppm	1.75	0.101	1.55	1.96	1.45	2.06	5.76%	11.53%	17.29%	1.67	1.84
Cu, wt. %	8.64	0.219	8.20	9.08	7.99	9.30	2.53%	5.06%	7.59%	8.21	9.07
Dy, ppm	4.54	0.48	3.57	5.50	3.08	5.99	10.67%	21.35%	32.02%	4.31	4.76
Er, ppm	2.70	0.51	1.68	3.71	1.18	4.22	18.81%	37.62%	56.43%	2.56	2.83
Eu, ppm	0.89	0.067	0.76	1.02	0.69	1.09	7.52%	15.04%	22.56%	0.85	0.93
Fe, wt. %	6.71	0.245	6.22	7.20	5.97	7.44	3.65%	7.30%	10.95%	6.37	7.04
Ga, ppm	28.1	1.30	25.5	30.7	24.2	32.0	4.64%	9.27%	13.91%	26.7	29.5
Gd, ppm	4.92	1.14	2.64	7.20	1.50	8.34	23.16%	46.31%	69.47%	4.68	5.17
Ge, ppm	0.23	0.03	0.17	0.29	0.14	0.32	13.44%	26.88%	40.32%	0.22	0.24
Hf, ppm	4.94	0.218	4.51	5.38	4.29	5.60	4.42%	8.83%	13.25%	4.70	5.19
Ho, ppm	0.89	0.18	0.52	1.26	0.33	1.44	20.80%	41.61%	62.41%	0.84	0.93
In, ppm	3.56	0.188	3.19	3.94	3.00	4.13	5.27%	10.54%	15.81%	3.39	3.74
K, wt. %	2.25	0.082	2.08	2.41	2.00	2.49	3.65%	7.31%	10.96%	2.13	2.36
La, ppm	70	4.3	61	78	57	83	6.22%	12.44%	18.66%	66	73
Li, ppm	52	2.7	46	57	44	60	5.18%	10.37%	15.55%	49	54
Lu, ppm	0.41	0.05	0.31	0.50	0.26	0.55	11.67%	23.34%	35.02%	0.39	0.43
Mg, wt. %	2.43	0.101	2.22	2.63	2.12	2.73	4.15%	8.30%	12.45%	2.30	2.55
Mn, wt. %	0.117	0.006	0.105	0.130	0.098	0.136	5.35%	10.70%	16.05%	0.111	0.123
Mo, ppm	18.4	0.97	16.4	20.3	15.5	21.2	5.26%	10.52%	15.78%	17.4	19.3
Na, wt. %	0.049	0.009	0.031	0.067	0.023	0.075	17.91%	35.83%	53.74%	0.047	0.051
Nb, ppm	14.0	2.4	9.2	18.8	6.8	21.2	17.11%	34.21%	51.32%	13.3	14.7
Nd, ppm	63	2.3	58	68	56	70	3.68%	7.36%	11.03%	60	66
Ni, ppm	337	19	300	374	281	393	5.53%	11.06%	16.60%	320	354
P, wt. %	0.033	0.002	0.028	0.037	0.026	0.040	7.24%	14.48%	21.71%	0.031	0.034
Pb, ppm	17.3	1.15	15.0	19.6	13.8	20.7	6.68%	13.36%	20.04%	16.4	18.1
Pr, ppm	16.5	1.62	13.3	19.8	11.7	21.4	9.82%	19.64%	29.46%	15.7	17.4
Rb, ppm	82	5.2	72	93	67	98	6.26%	12.52%	18.78%	78	86
Re, ppm	0.033	0.003	0.026	0.039	0.023	0.043	10.20%	20.39%	30.59%	0.031	0.034
S, wt. %	8.55	0.332	7.88	9.21	7.55	9.54	3.88%	7.76%	11.64%	8.12	8.97
Sb, ppm	5.29	0.473	4.35	6.24	3.87	6.71	8.94%	17.88%	26.83%	5.03	5.56
Sc, ppm	11.0	0.81	9.4	12.6	8.6	13.5	7.32%	14.64%	21.96%	10.5	11.6
Se, ppm	11.2	1.2	8.7	13.6	7.4	14.9	11.11%	22.21%	33.32%	10.6	11.7
Sm, ppm	8.58	0.573	7.43	9.72	6.86	10.30	6.67%	13.35%	20.02%	8.15	9.01
Sn, ppm	3.70	0.300	3.10	4.31	2.80	4.61	8.11%	16.22%	24.33%	3.52	3.89
Sr, ppm	68	3.0	61	74	58	77	4.51%	9.02%	13.53%	64	71
Ta, ppm	1.04	0.16	0.73	1.35	0.58	1.51	14.92%	29.85%	44.77%	0.99	1.09
Tb, ppm	0.78	0.17	0.45	1.11	0.28	1.28	21.35%	42.70%	64.05%	0.74	0.82
Te, ppm	0.089	0.023	0.044	0.135	0.021	0.158	25.57%	51.14%	76.71%	0.085	0.094
Th, ppm	15.4	0.87	13.7	17.2	12.8	18.0	5.62%	11.25%	16.87%	14.7	16.2
Ti, wt. %	0.235	0.051	0.133	0.337	0.082	0.389	21.77%	43.53%	65.30%	0.223	0.247
Tl, ppm	1.06	0.077	0.90	1.21	0.82	1.29	7.31%	14.61%	21.92%	1.00	1.11

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion continued											
Tm, ppm	0.39	0.04	0.31	0.48	0.26	0.52	11.05%	22.11%	33.16%	0.37	0.41
U, ppm	8.80	0.625	7.55	10.04	6.92	10.67	7.10%	14.20%	21.30%	8.36	9.24
V, ppm	330	17	297	364	280	380	5.05%	10.09%	15.14%	314	347
W, ppm	2.30	0.181	1.94	2.66	1.75	2.84	7.88%	15.76%	23.64%	2.18	2.41
Y, ppm	23.5	0.82	21.8	25.1	21.0	25.9	3.50%	7.01%	10.51%	22.3	24.6
Yb, ppm	2.72	0.34	2.04	3.41	1.70	3.75	12.55%	25.11%	37.66%	2.59	2.86
Zn, ppm	38.8	2.61	33.6	44.0	31.0	46.6	6.73%	13.47%	20.20%	36.9	40.7
Zr, ppm	171	6	158	184	152	190	3.68%	7.37%	11.05%	163	180
Aqua Regia Digestion											
Ag, ppm	0.120	0.017	0.086	0.153	0.069	0.170	14.01%	28.01%	42.02%	0.114	0.126
Al, wt. %	0.869	0.144	0.580	1.158	0.436	1.303	16.62%	33.25%	49.87%	0.826	0.913
As, ppm	94	6.3	81	107	75	113	6.71%	13.41%	20.12%	89	99
Au, ppm	< 0.02	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
B, ppm	< 10	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Ba, ppm	53	13	26	79	13	92	24.86%	49.73%	74.59%	50	55
Be, ppm	2.20	0.25	1.70	2.71	1.45	2.96	11.42%	22.85%	34.27%	2.09	2.31
Bi, ppm	2.82	0.182	2.45	3.18	2.27	3.36	6.45%	12.91%	19.36%	2.68	2.96
Ca, wt. %	0.131	0.003	0.124	0.137	0.120	0.141	2.62%	5.25%	7.87%	0.124	0.137
Cd, ppm	0.51	0.029	0.45	0.57	0.42	0.60	5.60%	11.19%	16.79%	0.48	0.54
Ce, ppm	43.6	6.0	31.6	55.6	25.6	61.6	13.77%	27.54%	41.31%	41.4	45.8
Co, wt. %	1.98	0.076	1.82	2.13	1.75	2.21	3.87%	7.74%	11.61%	1.88	2.08
Cr, ppm	35.0	2.23	30.5	39.5	28.3	41.7	6.37%	12.74%	19.11%	33.3	36.8
Cs, ppm	0.29	0.10	0.10	0.49	0.01	0.58	32.65%	65.31%	97.96%	0.28	0.31
Cu, wt. %	8.55	0.181	8.19	8.92	8.01	9.10	2.12%	4.24%	6.36%	8.13	8.98
Dy, ppm	1.02	0.11	0.80	1.23	0.69	1.34	10.62%	21.24%	31.86%	0.96	1.07
Er, ppm	0.41	0.09	0.23	0.59	0.14	0.68	21.89%	43.79%	65.68%	0.39	0.43
Eu, ppm	0.38	0.035	0.31	0.45	0.28	0.49	9.16%	18.32%	27.48%	0.36	0.40
Fe, wt. %	6.65	0.197	6.25	7.04	6.05	7.24	2.96%	5.92%	8.89%	6.31	6.98
Ga, ppm	9.61	1.62	6.38	12.85	4.76	14.46	16.82%	33.65%	50.47%	9.13	10.09
Gd, ppm	1.91	0.20	1.51	2.32	1.31	2.52	10.58%	21.16%	31.74%	1.82	2.01
Ge, ppm	0.13	0.03	0.07	0.19	0.04	0.21	23.65%	47.29%	70.94%	0.12	0.13
Hf, ppm	0.37	0.04	0.29	0.44	0.25	0.48	10.59%	21.19%	31.78%	0.35	0.39
Hg, ppm	0.11	0.02	0.07	0.14	0.05	0.16	16.37%	32.74%	49.12%	0.10	0.11
Ho, ppm	0.17	0.03	0.11	0.23	0.07	0.26	18.40%	36.80%	55.20%	0.16	0.18
In, ppm	2.94	0.184	2.57	3.30	2.38	3.49	6.26%	12.52%	18.78%	2.79	3.08
K, wt. %	0.187	0.028	0.132	0.243	0.104	0.270	14.77%	29.54%	44.31%	0.178	0.197
La, ppm	19.5	3.0	13.5	25.4	10.6	28.4	15.24%	30.49%	45.73%	18.5	20.4
Li, ppm	31.2	6.3	18.7	43.7	12.5	50.0	20.03%	40.06%	60.09%	29.7	32.8
Mg, wt. %	1.85	0.21	1.42	2.27	1.21	2.48	11.44%	22.89%	34.33%	1.76	1.94
Mn, wt. %	0.117	0.005	0.106	0.127	0.101	0.132	4.40%	8.81%	13.21%	0.111	0.123
Mo, ppm	17.4	1.15	15.1	19.7	13.9	20.8	6.60%	13.20%	19.79%	16.5	18.2
Na, wt. %	0.016	0.005	0.007	0.025	0.003	0.030	27.82%	55.64%	83.45%	0.015	0.017
Nb, ppm	0.13	0.03	0.06	0.19	0.02	0.23	27.25%	54.50%	81.75%	0.12	0.13
Nd, ppm	23.0	3.5	16.0	30.0	12.5	33.4	15.21%	30.42%	45.63%	21.8	24.1

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Aqua Regia Digestion continued											
Ni, ppm	323	23	277	370	253	393	7.21%	14.43%	21.64%	307	339
P, wt. %	0.019	0.002	0.015	0.022	0.014	0.024	8.98%	17.97%	26.95%	0.018	0.020
Pb, ppm	14.9	0.83	13.2	16.5	12.4	17.3	5.56%	11.12%	16.68%	14.1	15.6
Pr, ppm	5.75	0.87	4.01	7.50	3.14	8.37	15.16%	30.33%	45.49%	5.47	6.04
Rb, ppm	6.10	1.09	3.92	8.27	2.84	9.36	17.82%	35.65%	53.47%	5.79	6.40
Re, ppm	0.029	0.002	0.025	0.034	0.022	0.036	8.12%	16.23%	24.35%	0.028	0.031
S, wt. %	8.38	0.523	7.33	9.43	6.81	9.95	6.24%	12.49%	18.73%	7.96	8.80
Sb, ppm	3.32	0.312	2.70	3.95	2.39	4.26	9.38%	18.75%	28.13%	3.16	3.49
Sc, ppm	2.76	0.31	2.14	3.38	1.83	3.69	11.19%	22.38%	33.58%	2.62	2.90
Se, ppm	10.8	1.8	7.2	14.4	5.4	16.2	16.68%	33.37%	50.05%	10.3	11.3
Sm, ppm	3.50	0.45	2.59	4.41	2.14	4.86	12.93%	25.87%	38.80%	3.33	3.68
Sn, ppm	2.45	0.103	2.25	2.66	2.14	2.76	4.20%	8.40%	12.60%	2.33	2.57
Sr, ppm	15.4	3.0	9.4	21.5	6.3	24.5	19.65%	39.31%	58.96%	14.7	16.2
Ta, ppm	< 0.01	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Tb, ppm	0.20	0.04	0.13	0.28	0.09	0.32	18.54%	37.08%	55.62%	0.19	0.21
Te, ppm	0.075	0.015	0.046	0.105	0.031	0.119	19.55%	39.11%	58.66%	0.071	0.079
Th, ppm	6.16	0.94	4.29	8.04	3.35	8.98	15.24%	30.48%	45.72%	5.86	6.47
U, ppm	3.57	0.265	3.04	4.10	2.77	4.36	7.42%	14.84%	22.26%	3.39	3.75
V, ppm	60	8	45	76	37	83	12.69%	25.38%	38.07%	57	63
W, ppm	0.98	0.094	0.79	1.17	0.70	1.27	9.58%	19.17%	28.75%	0.93	1.03
Y, ppm	4.03	0.46	3.11	4.94	2.65	5.40	11.39%	22.79%	34.18%	3.82	4.23
Yb, ppm	0.38	0.06	0.26	0.51	0.19	0.57	16.62%	33.24%	49.86%	0.36	0.40
Zn, ppm	37.1	2.38	32.4	41.9	30.0	44.3	6.40%	12.81%	19.21%	35.3	39.0
Zr, ppm	11.1	1.6	7.9	14.2	6.3	15.8	14.28%	28.55%	42.83%	10.5	11.6

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

PARTICIPATING LABORATORIES

1. Actlabs, Ancaster, Ontario, Canada
2. African Natural Resources & Mines Ltd, Suleja, Niger State, Nigeria
3. AGAT Laboratories, Calgary, Alberta, Canada
4. ALS, Brisbane, QLD, Australia
5. ALS, Lima, Peru
6. ALS, Loughrea, Galway, Ireland
7. ALS, Malaga, WA, Australia
8. ALS, Vancouver, BC, Canada
9. American Assay Laboratories, Sparks, Nevada, USA
10. ARGETEST Mineral Processing, Ankara, Central Anatolia, Turkey
11. Bureau Veritas Commodities Canada Ltd, Vancouver, BC, Canada
12. CERTIMIN, Lima, Peru
13. ESAN Istanbul, Istanbul, Turkey
14. Inspectorate (BV), Lima, Peru
15. Intertek Genalysis, Perth, WA, Australia
16. Intertek Testing Services, Townsville, QLD, Australia
17. Intertek Testing Services Philippines, Cupang, Muntinlupa, Philippines
18. Labwest Minerals Analysis, Perth, WA, Australia
19. MSALABS, Vancouver, BC, Canada
20. Ontario Geological Survey, Sudbury, Ontario, Canada
21. PT Geoservices Ltd, Cikarang, Jakarta Raya, Indonesia
22. PT Intertek Utama Services, Jakarta Timur, DKI Jakarta, Indonesia
23. Saskatchewan Research Council, Saskatoon, Saskatchewan, Canada
24. SGS, Randfontein, Gauteng, South Africa
25. SGS del Peru, Lima, Peru
26. Shiva Analyticals Ltd, Bangalore North, Karnataka, India
27. Skyline Assayers & Laboratories, Tucson, Arizona, USA
28. Stewart Assay & Environmental Laboratories LLC, Kara-Balta, Chüy, Kyrgyzstan

Please note: To preserve anonymity, the above numbered alphabetical list of participating laboratories does not correspond with the Lab ID numbering on the scatter plots below.

PREPARER AND SUPPLIER

Certified reference material OREAS 556b is prepared, certified and supplied by:



ORE Research & Exploration Pty Ltd
37A Hosie Street
Bayswater North VIC 3153
AUSTRALIA

Tel: +613-9729 0333
Fax: +613-9729 8338
Web: www.oreas.com
Email: info@ore.com.au

Figure 1. Co by Borate Fusion XRF in OREAS 556b

SPC.1785.RR1.OREAS 556b.1.Fusion XRF.Co.Lab.240205.163501.SN

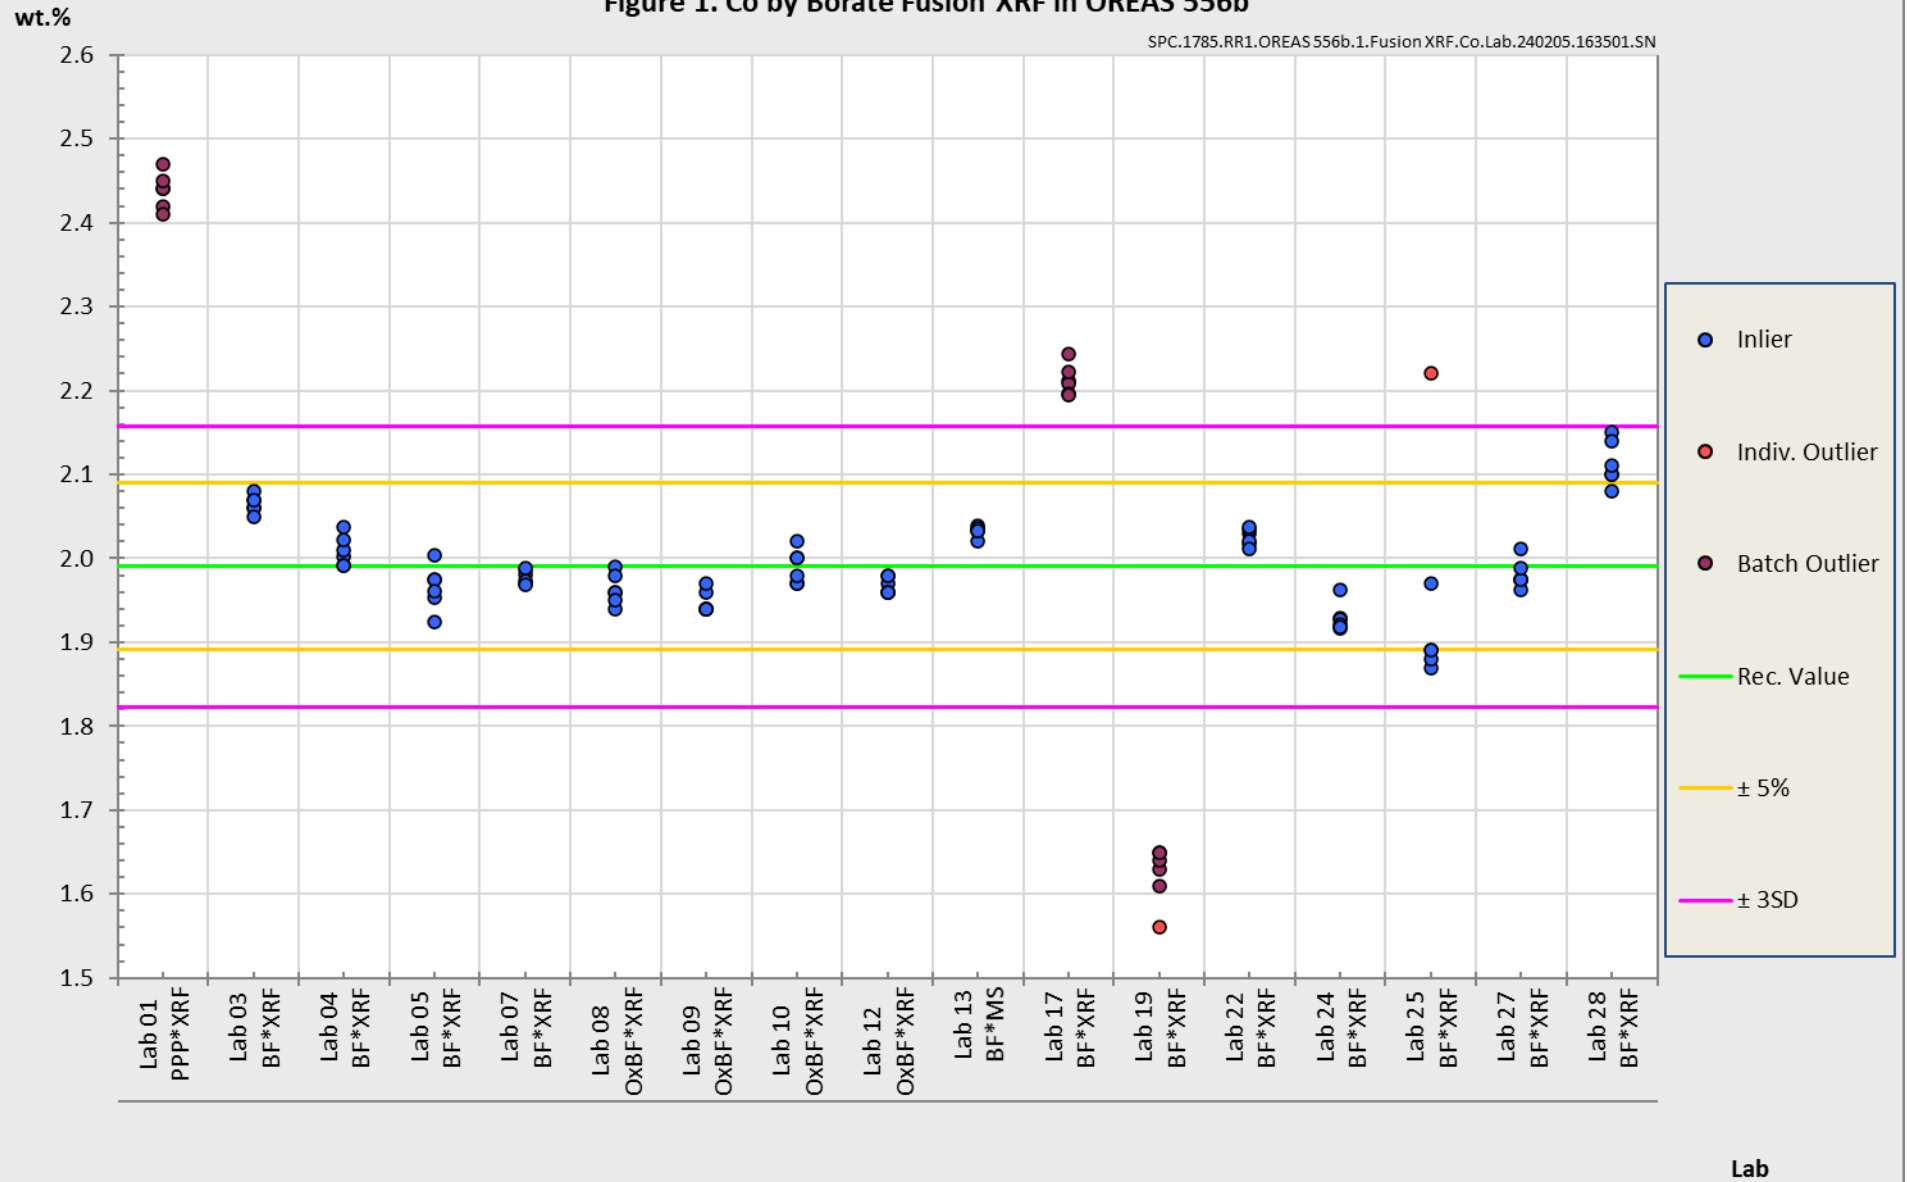


Figure 2. Cu by Borate Fusion XRF in OREAS 556b

SPC.1785.RR1.OREAS556b.1.Fusion XRF.Cu.Lab.240212.131102.SS

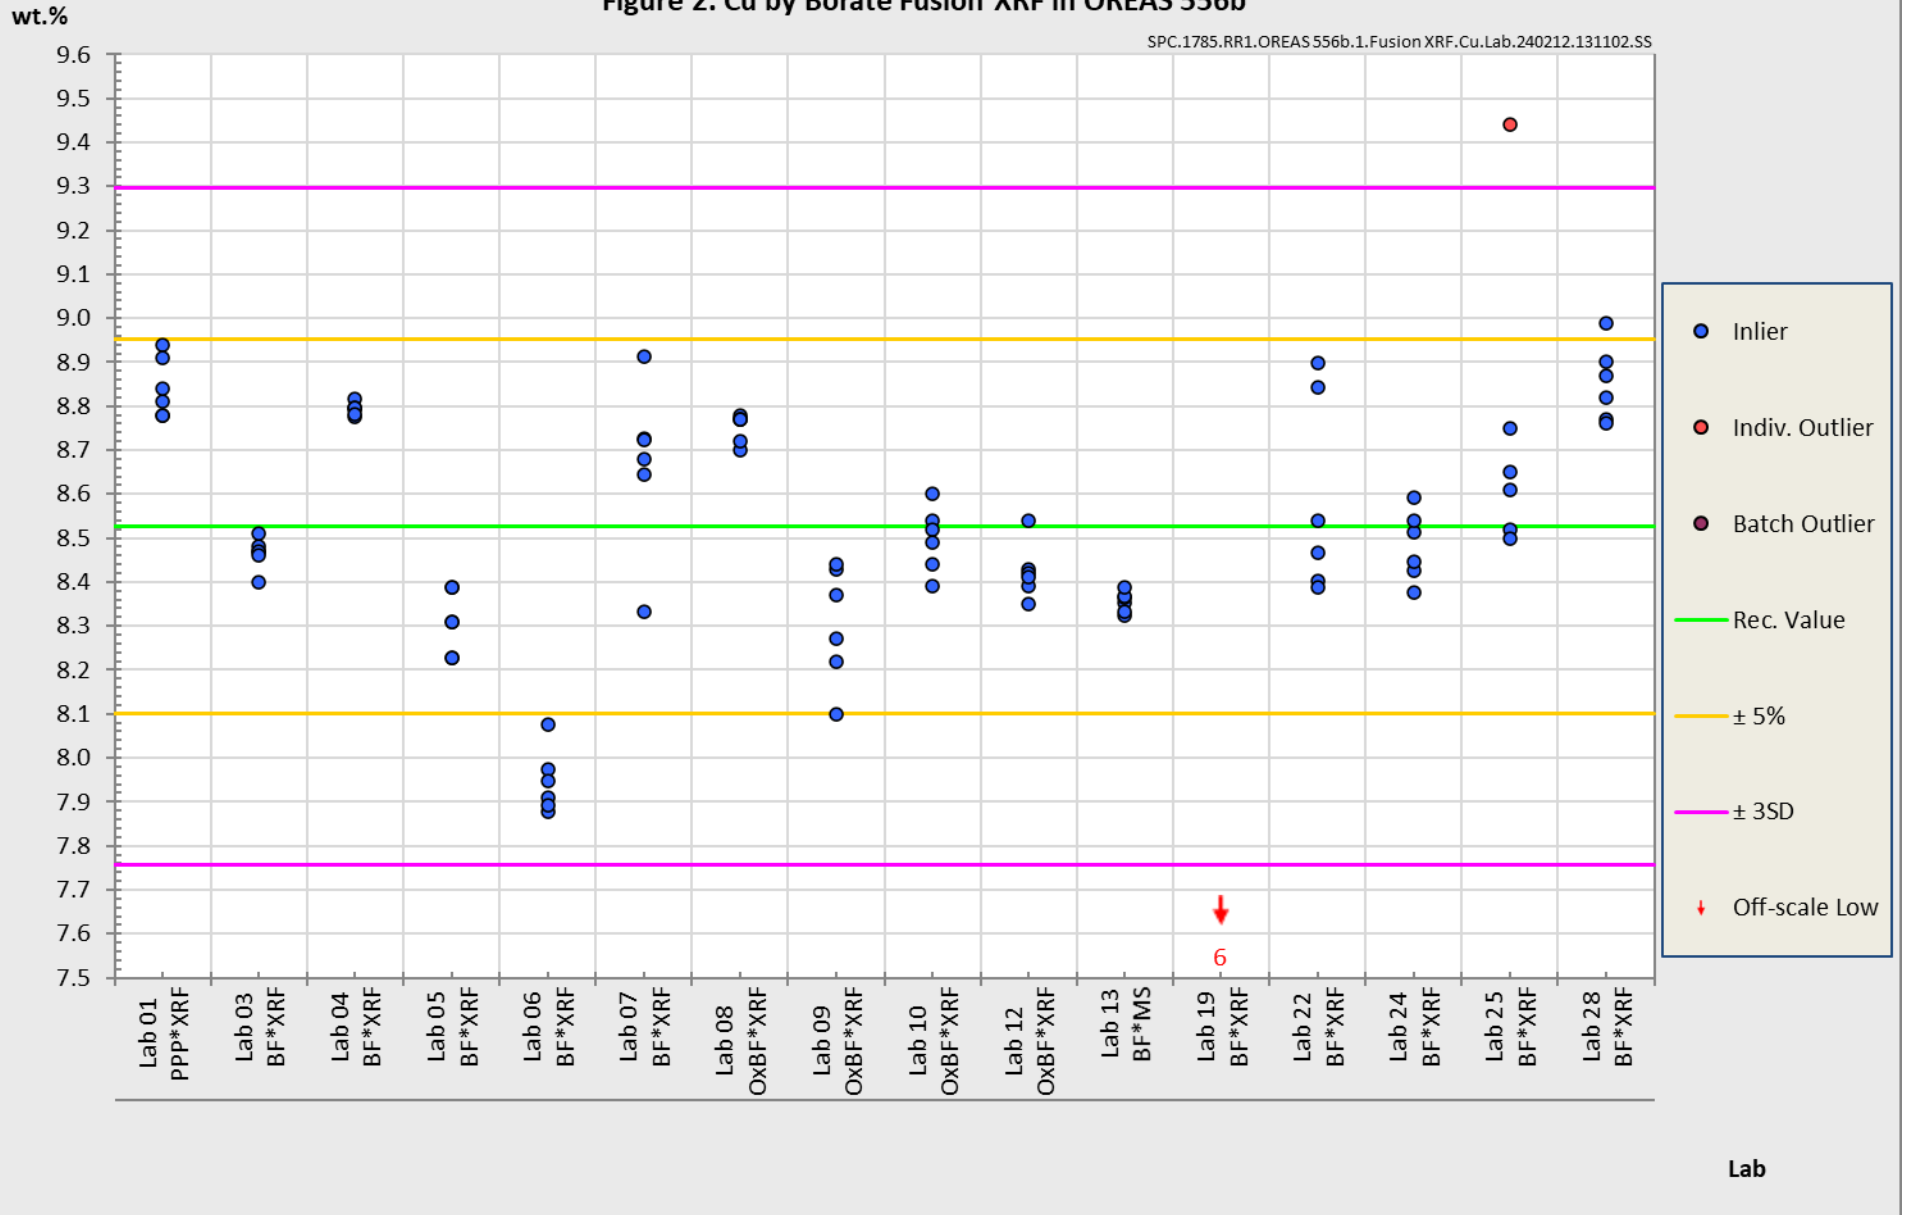


Figure 3. Co by Peroxide Fusion ICP in OREAS 556b

SPC.1785.RR1.OREAS556b.1.PF ICP.Co.Lab.240205.164048.SN

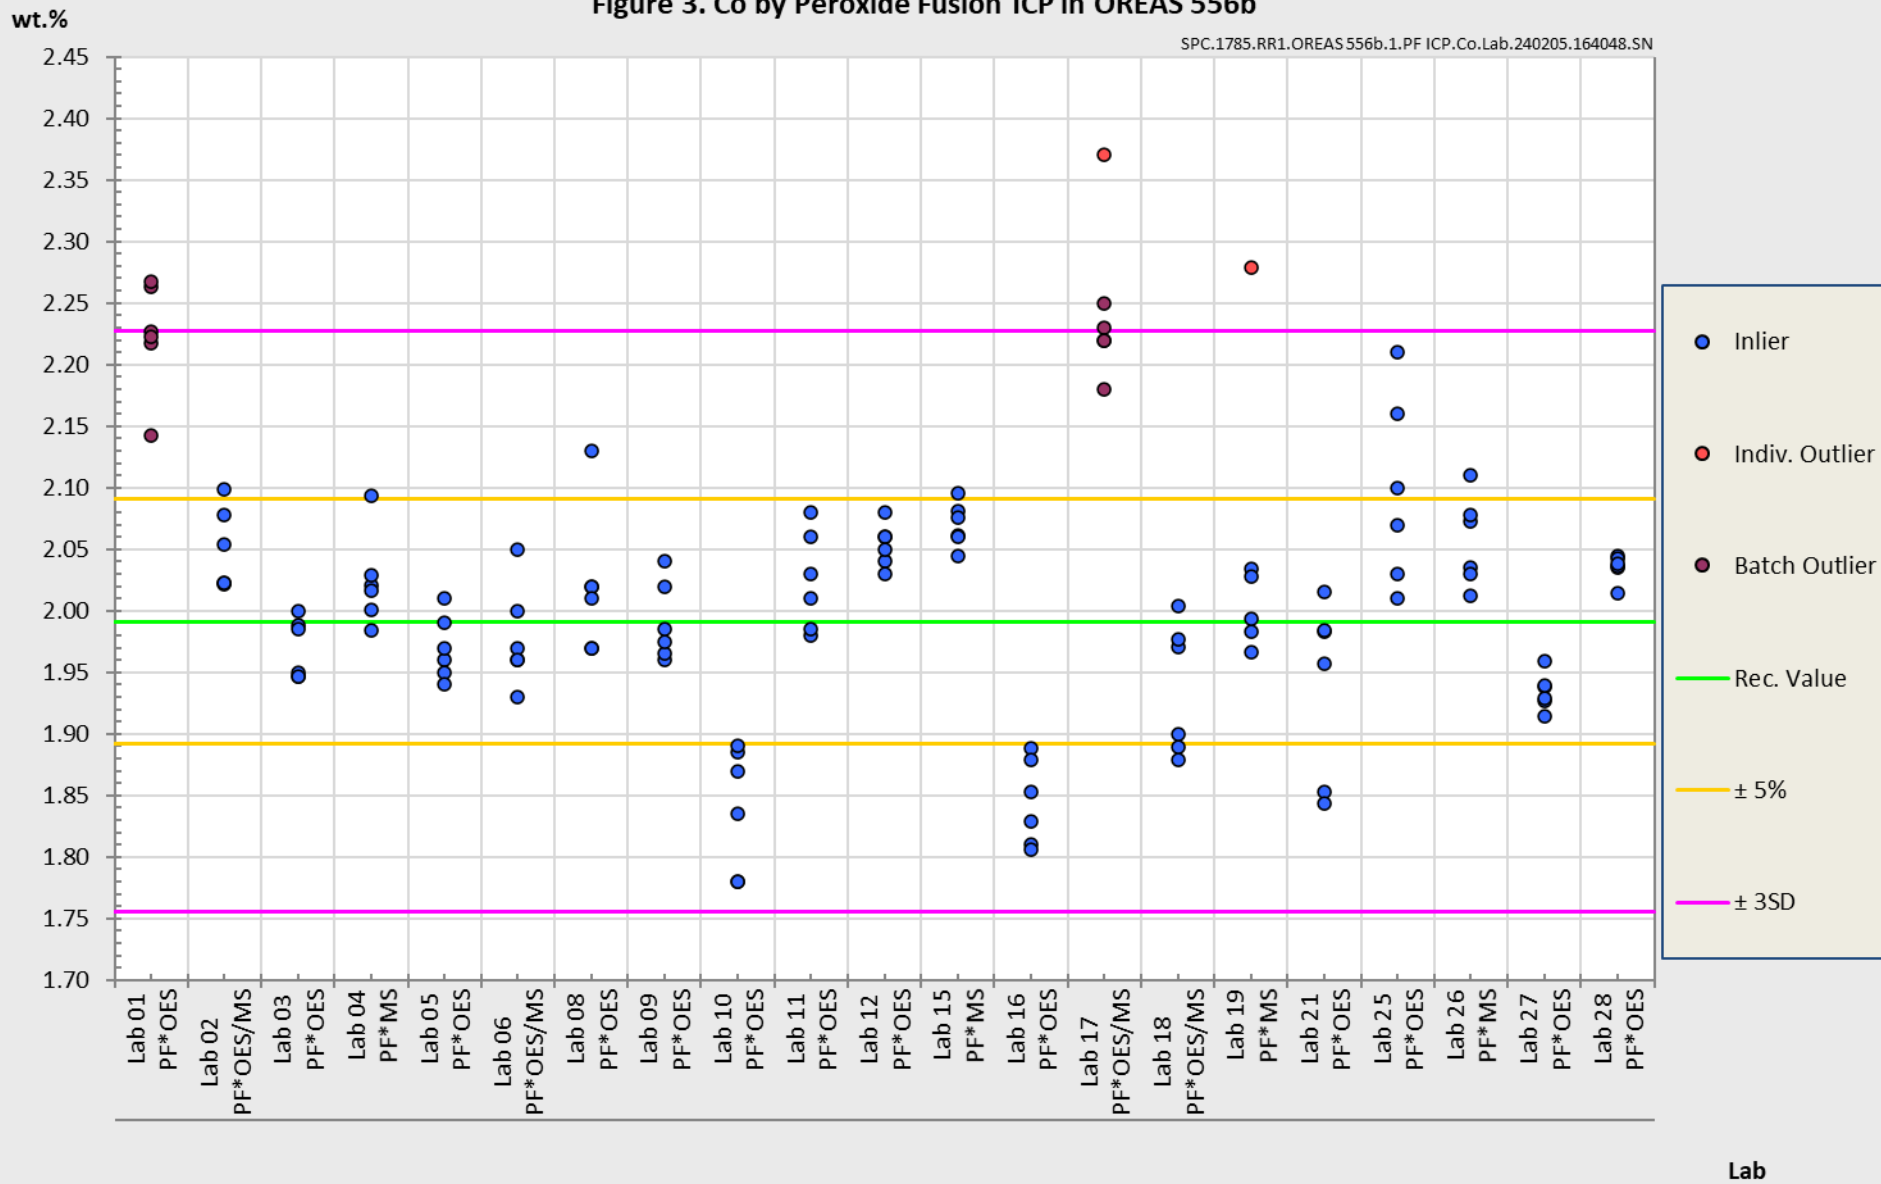


Figure 4. Cu by Peroxide Fusion ICP in OREAS 556b

SPC.1785.RR1.OREAS 556b.1.PF ICP.Cu.Lab.240215.141037.SN

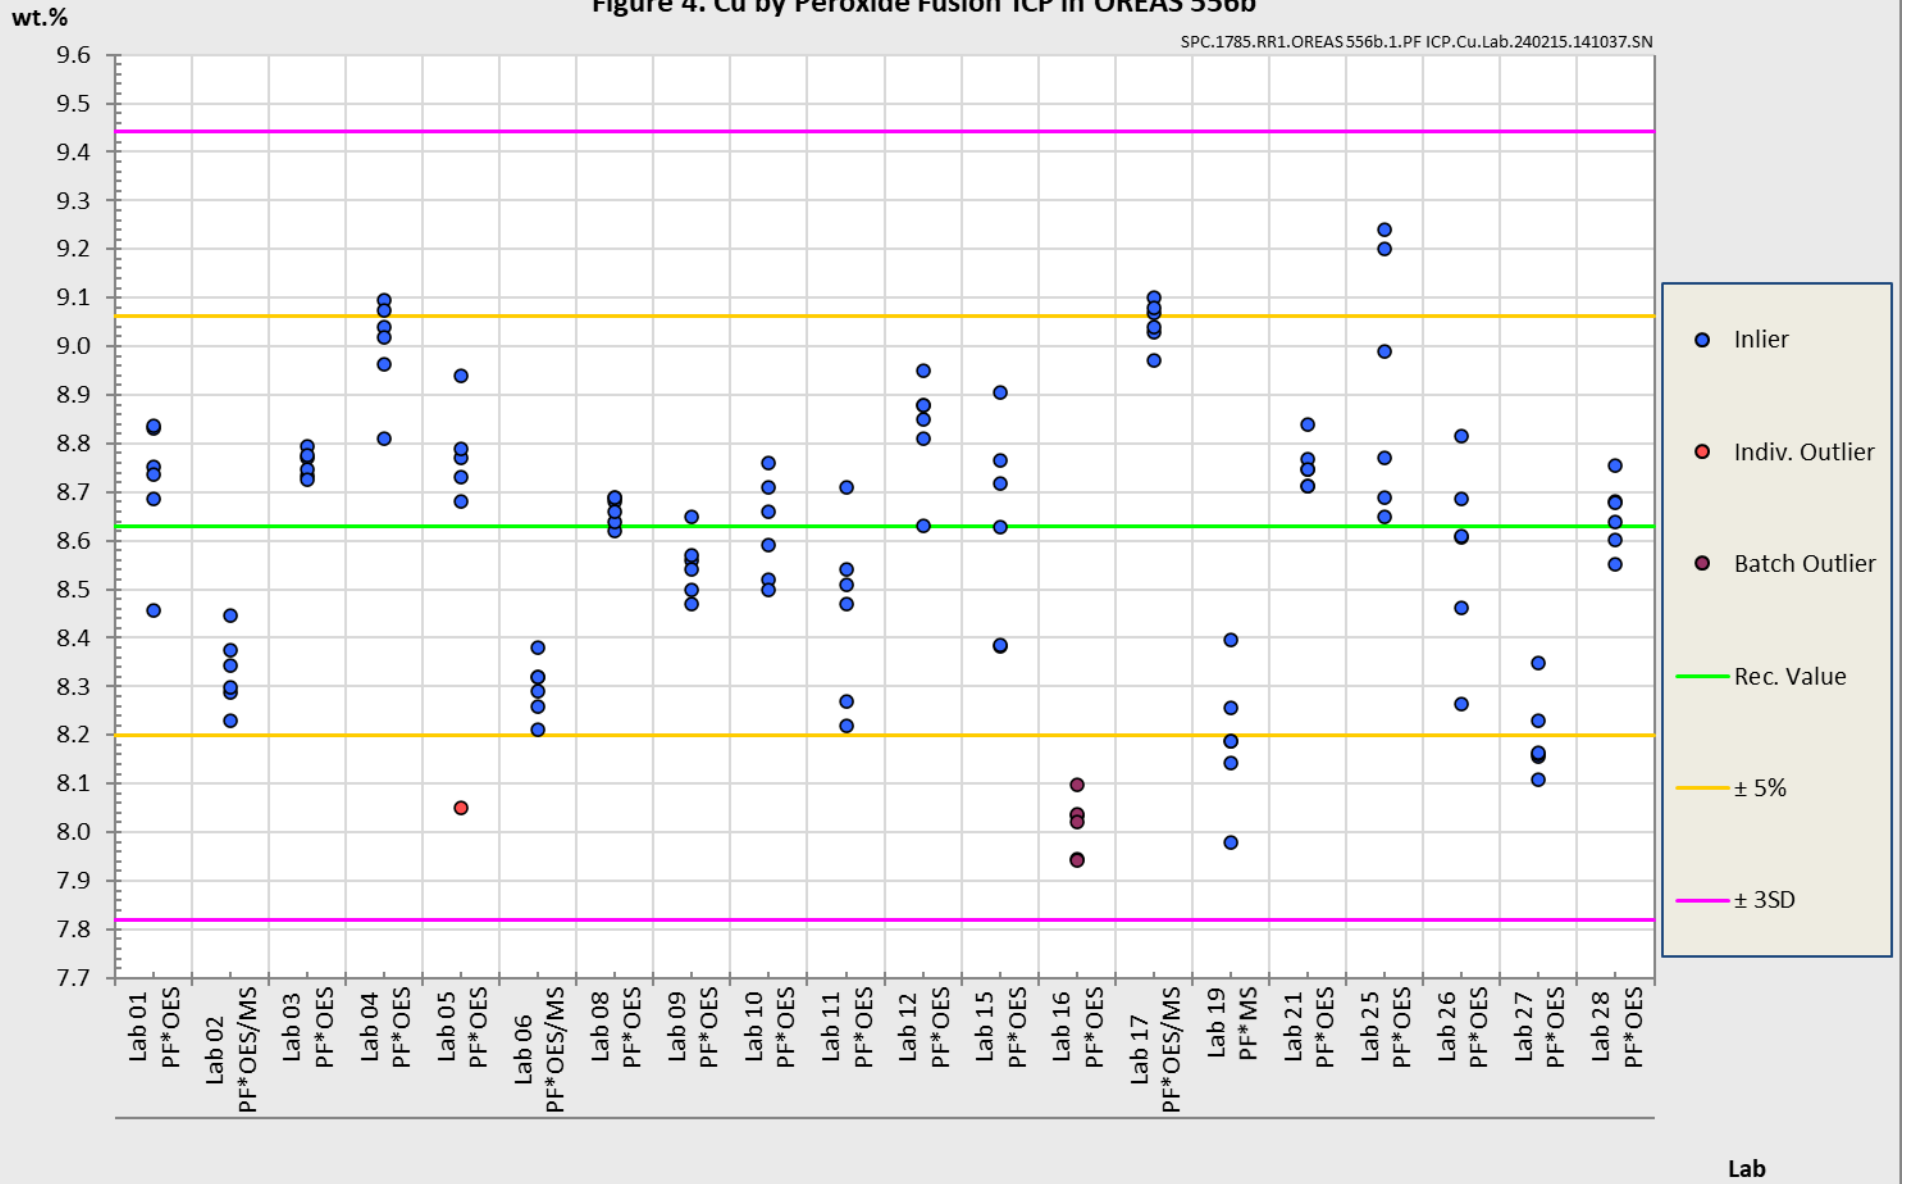


Figure 5. Co by 4-Acid Digestion in OREAS 556b

SPC.1785.RR1.OREAS 556b.1.4-Acid.Co.Lab.240205.164323.SS

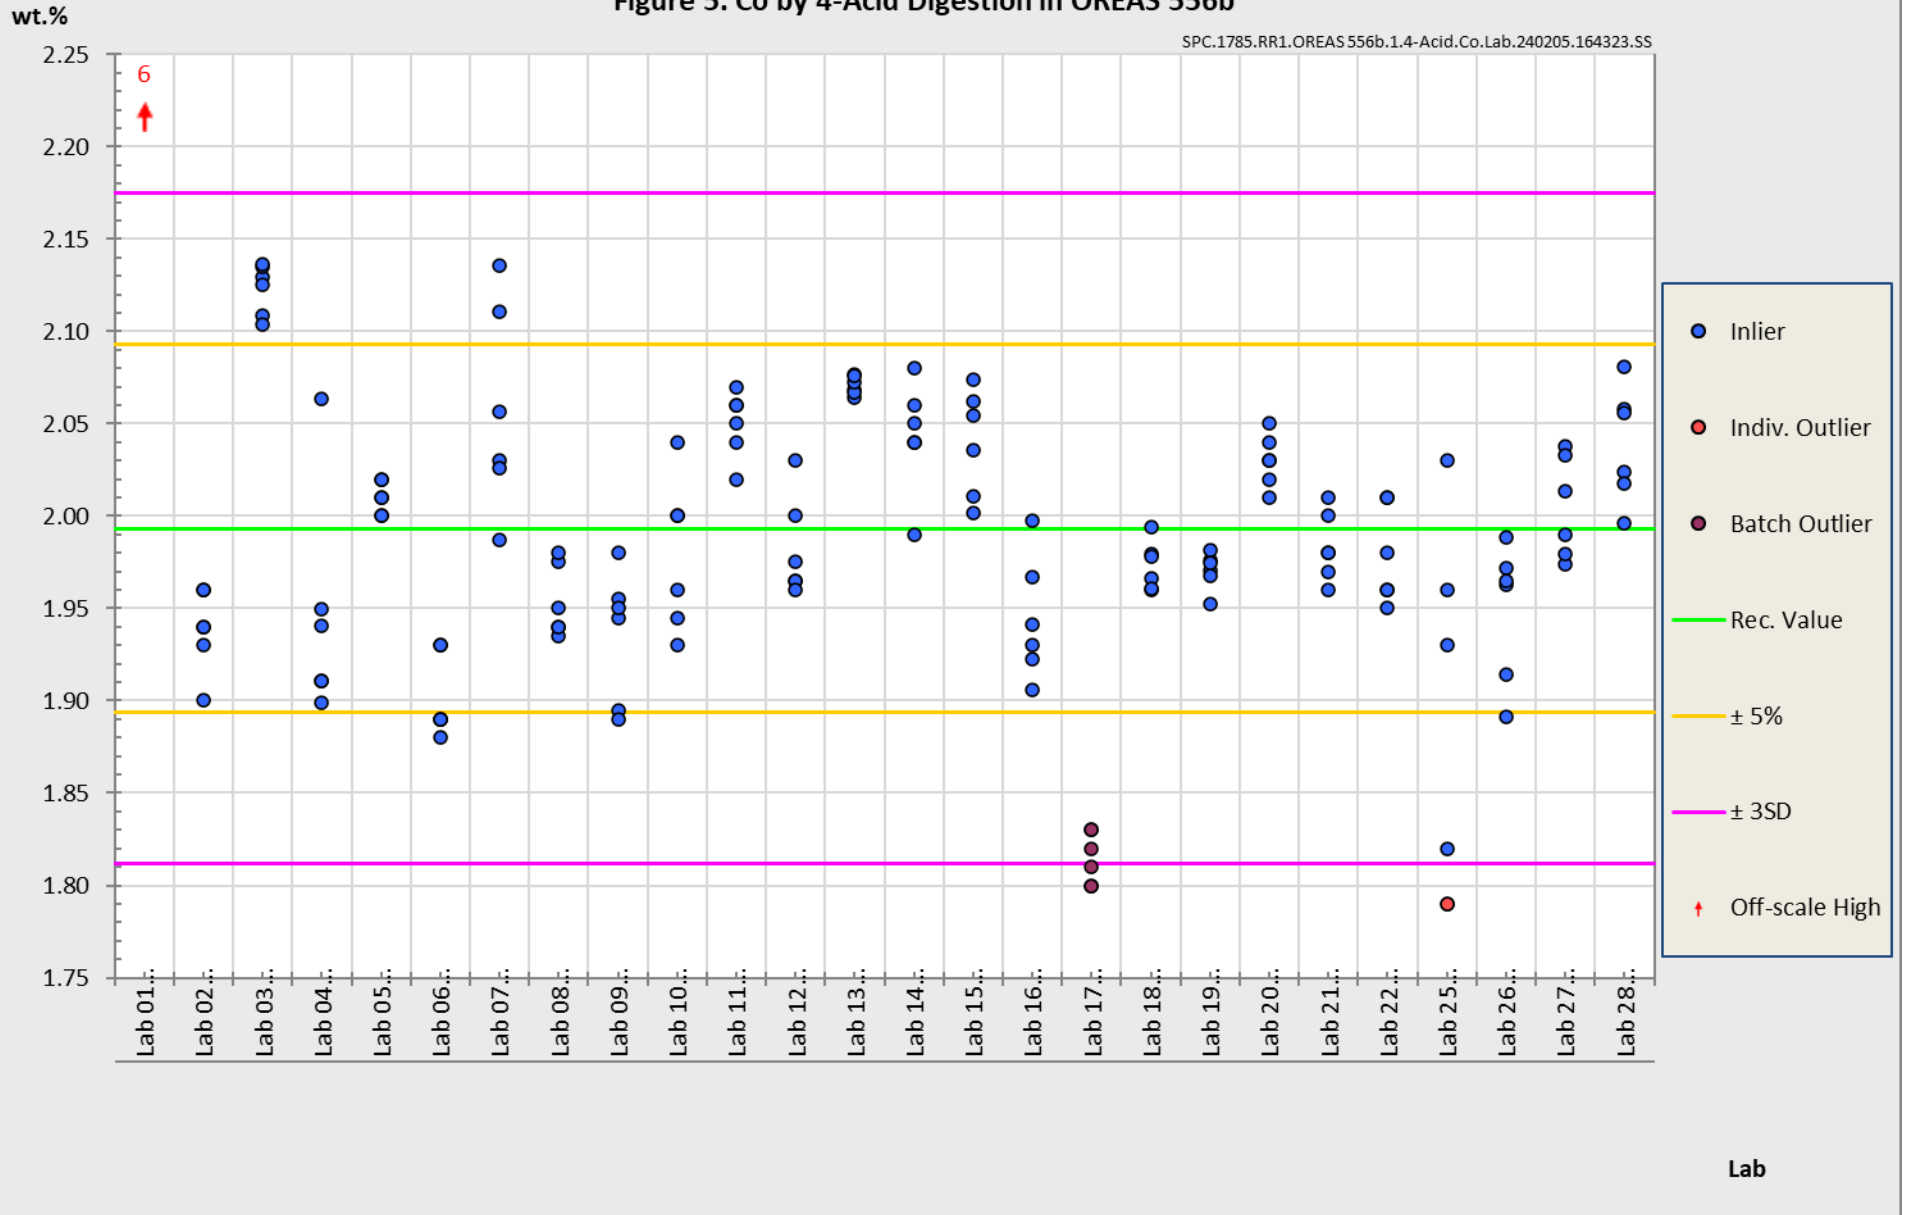


Figure 6. Cu by 4-Acid Digestion in OREAS 556b

SPC.1785.RR1.OREAS 556b.1.4-Acid.Cu.Lab.240205.170725.SS

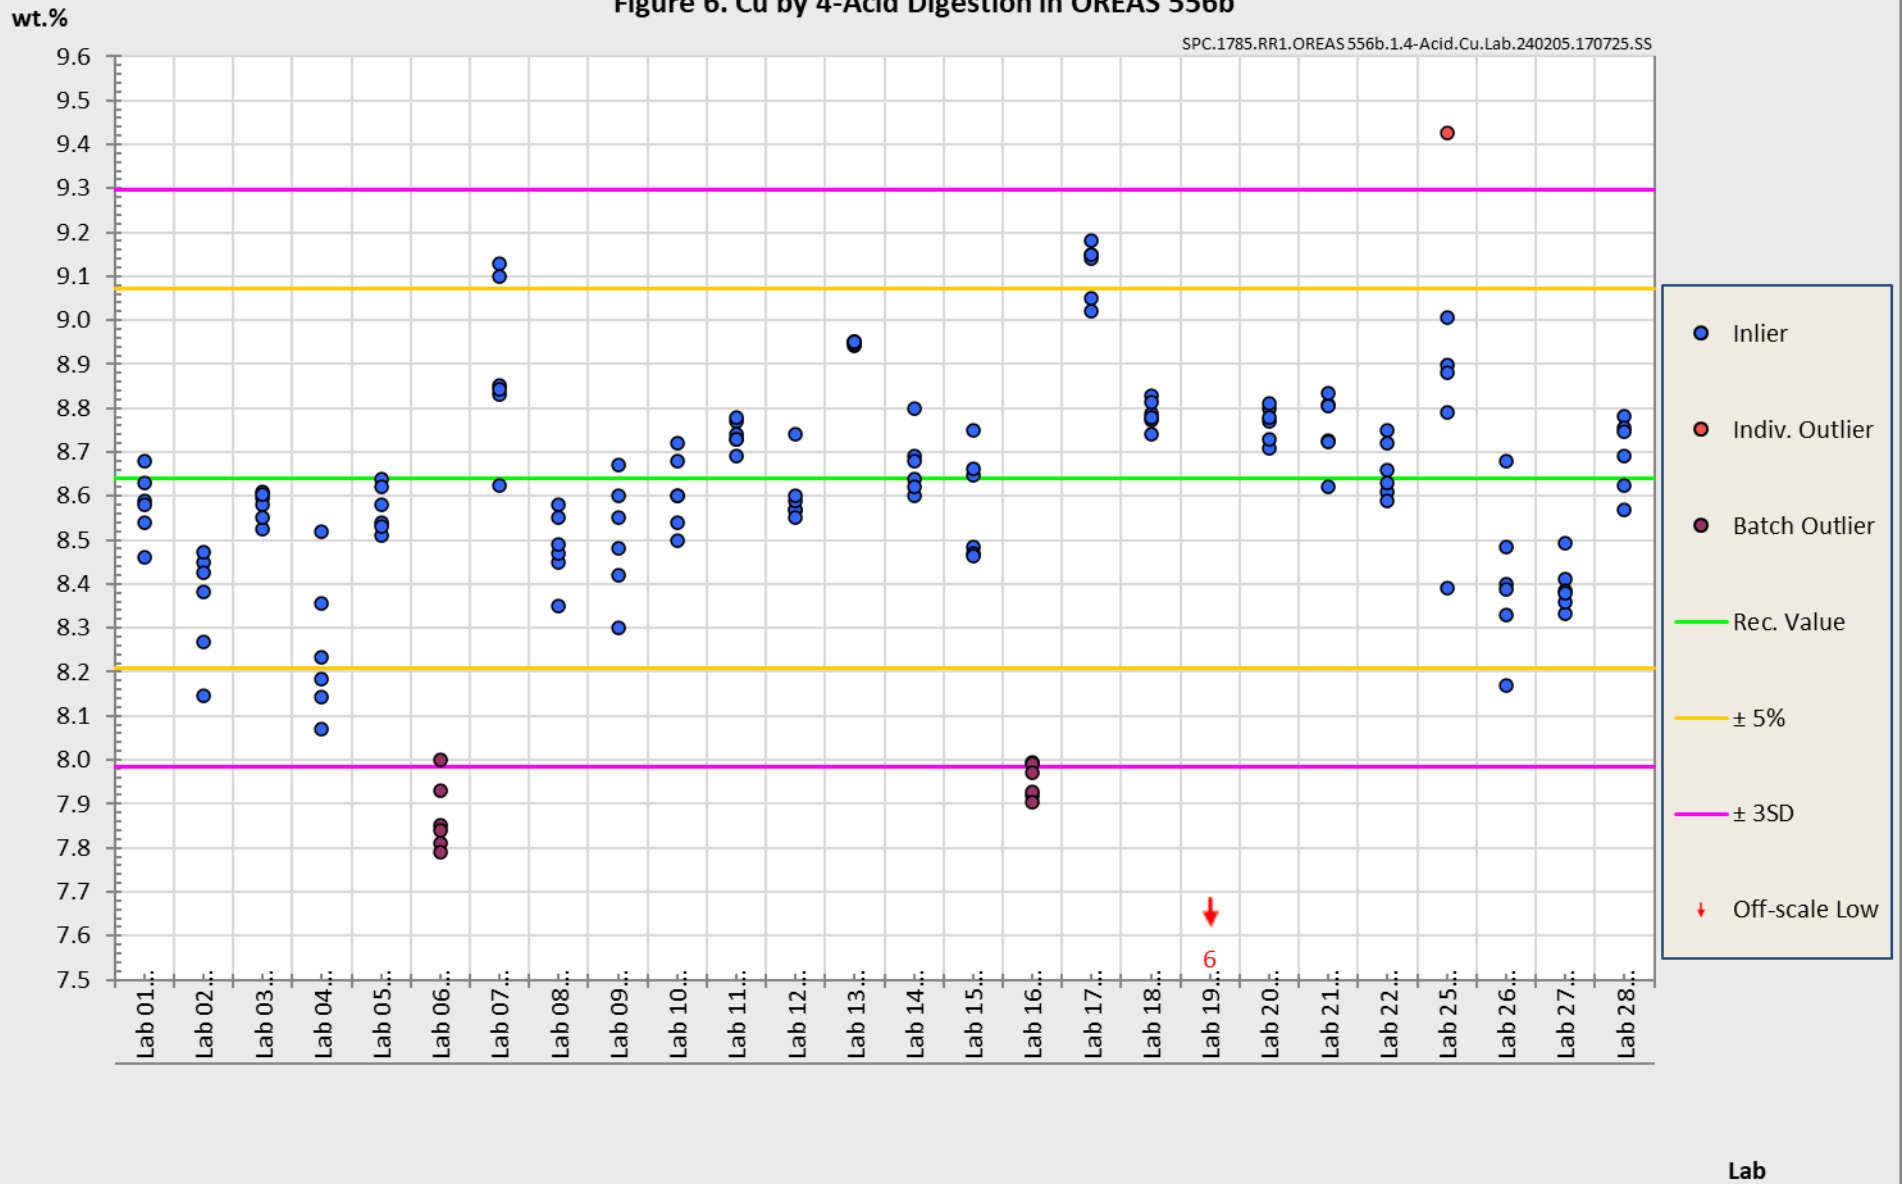


Figure 7. Co by Aqua Regia Digestion in OREAS 556b

SPC.1785.RR1.OREAS 556b.1.Aqua Regia.Co.Lab.240205.164430.SN


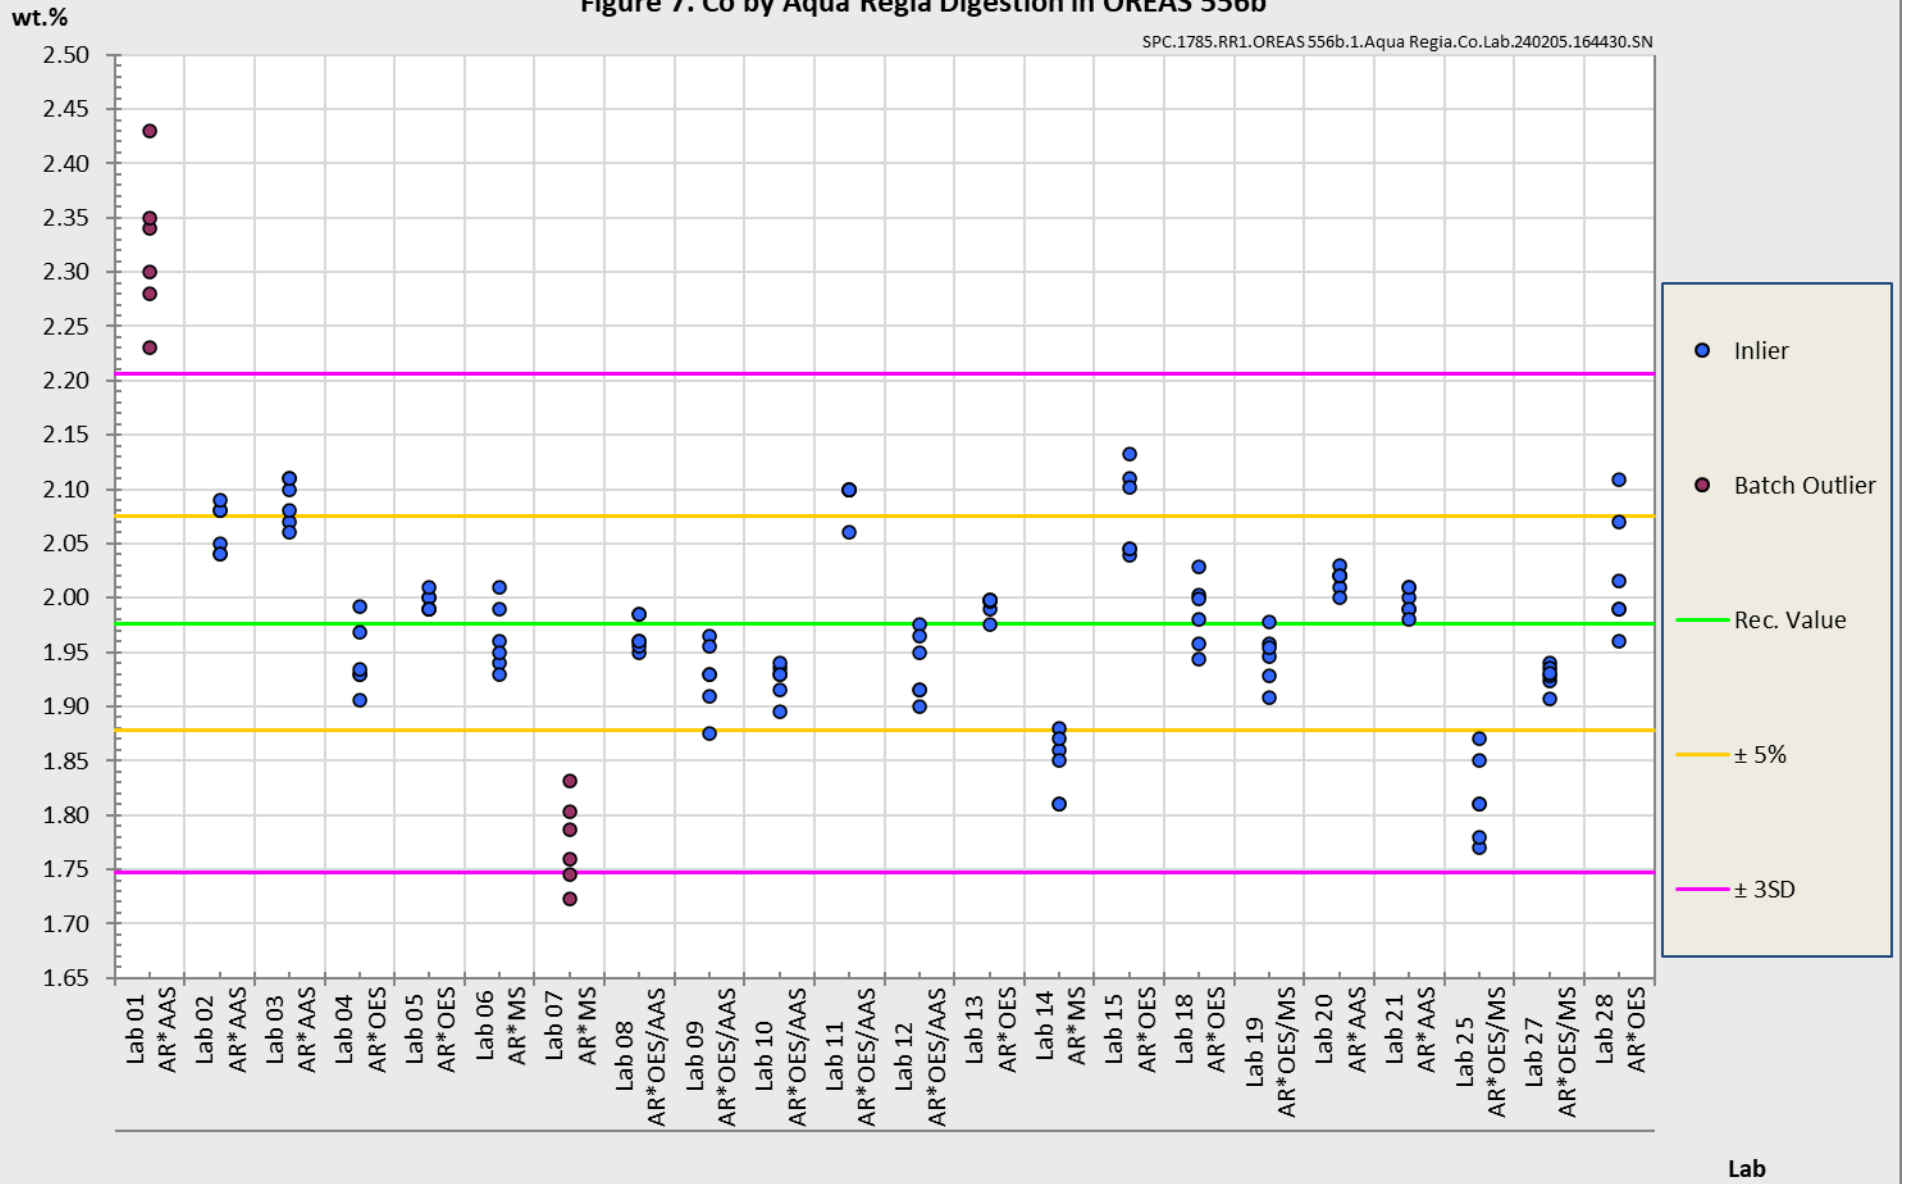


Figure 8. Cu by Aqua Regia Digestion in OREAS 556b

SPC.1785.RR1.OREAS556b.1.Aqua Regia.Cu.Lab.240205.171009.SS

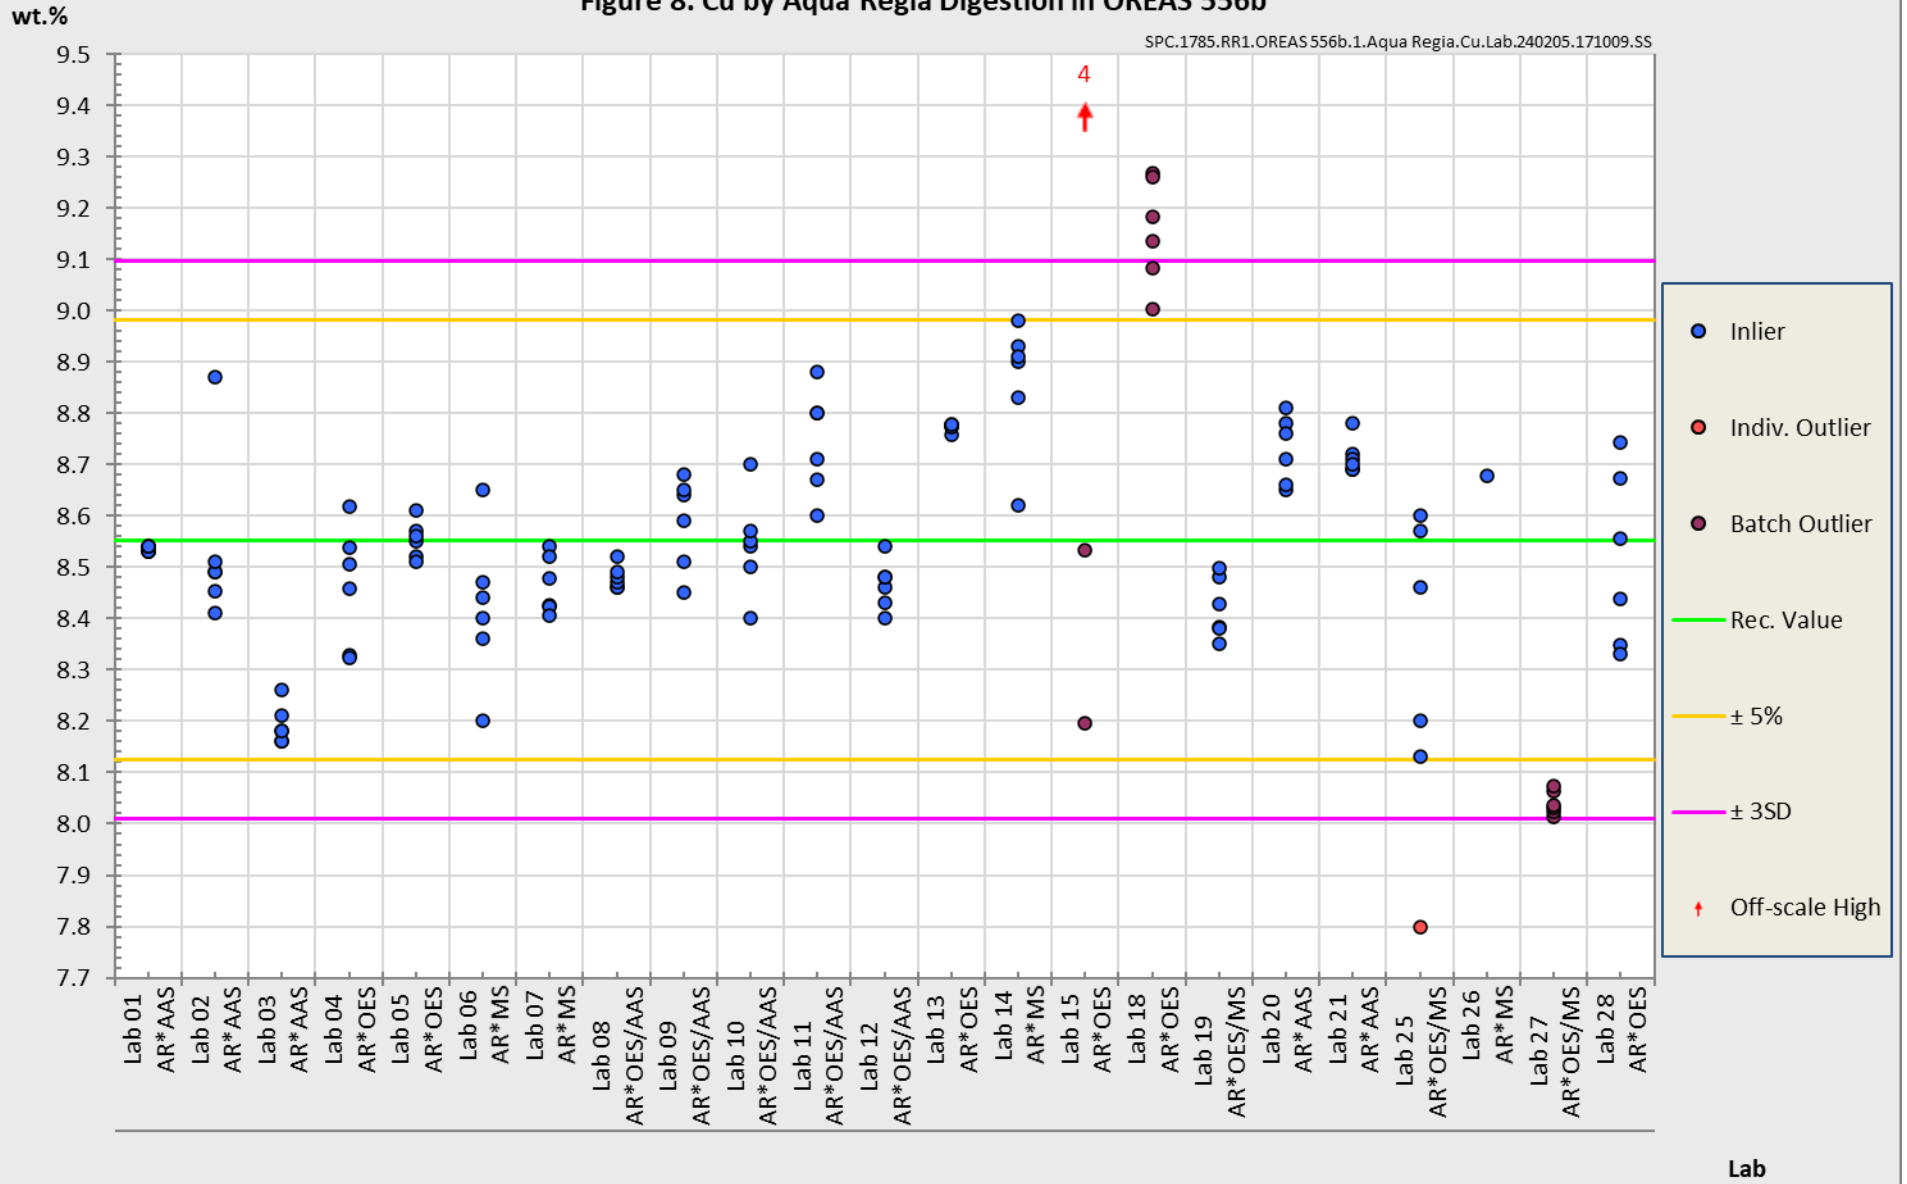

METROLOGICAL TRACEABILITY

The interlaboratory results that underpin the certified values are metrologically traceable to the international measurement scale (SI) of mass (either as a % mass fraction or as milligrams per kilogram (mg/kg)). In line with popular use, all data within tables in this certificate are expressed as the mass fraction in either weight percent (wt.%) or parts per million (ppm).

The analytical samples sent to participating laboratories were selected in a manner to be representative of the entire prepared batch of CRM. This 'representivity' was maintained in each submitted laboratory sample batch and ensures the user that the data is traceable from sample selection through to the analytical results. The systematic sampling method was chosen due to the low risk of overlooking repetitive effects or trends in the batch due to the way the CRM was processed. In line with ISO 17025 [8], each analytical data set received from the participating laboratories has been validated by its assayer through the inclusion of internal reference materials and QC checks during and post analysis.

The participating laboratories were chosen on the basis of their competence (from past performance in interlaboratory programs undertaken by ORE Pty Ltd) for a particular analytical method, analyte or analyte suite and sample matrix. These laboratories are accredited to ISO 17025 for 4-acid digestion and aqua regia digestion methods (Table 1). The other operationally defined measurands characterised in this certificate (Table 2) are derived from data procured mostly from ISO 17025 accredited laboratories. The certified values presented in this report are calculated from the means of accepted data following robust technical and statistical analysis as detailed in this report.

Guide ISO/TR 16476:2016, section 5.3.1 describes metrological traceability in reference materials as it pertains to the transformation of the measurand. In this section it states, *"Although the determination of the property value itself can be made traceable to appropriate units through, for example, calibration of the measurement equipment used, steps like the transformation of the sample from one physical (chemical) state to another cannot. Such transformations may only be compared with a reference (when available), or among themselves. For some transformations, reference methods have been defined and may be used in certification projects to evaluate the uncertainty associated with such a transformation. In other cases, only a comparison among different laboratories using the same procedure is possible. In this case, it is impossible to demonstrate absence of method bias; therefore, the result is an operationally defined measurand (ISO Guide 35:2017, 9.2.4c)."* Certification takes place on the basis of agreement among operationally defined, independent measurement results.

COMMUTABILITY

The measurements of the results that underlie the certified values contained in this report were undertaken by methods involving pre-treatment (fusion/digestion) of the sample. This served to reduce the sample to a simple and well understood form permitting calibration using simple solutions of the CRM. Due to these methods being well understood and highly effective, commutability is not an issue for this CRM. All OREAS CRMs are sourced from natural ore minerals meaning they will display similar behaviour as routine 'field' samples in the relevant measurement process. Care should be taken to ensure 'matrix matching' as close as practically achievable. The matrix and mineralisation style of the CRM is described in the 'Source Material' section and users should select appropriate CRMs matching these attributes to the field samples being analysed.

INTENDED USE

OREAS 556b is intended to cover all activities needed to produce a measurement result. This includes extraction, possible separation steps and the actual measurement process (the signal producing step). OREAS 556b may be used to calibrate the entire procedure by producing a pure substance CRM transformed into a calibration solution.

OREAS 556b is intended for the following uses:

- For the monitoring of laboratory performance in the analysis of analytes reported in Tables 1 and 2 in geological samples;
- For the verification of analytical methods for analytes reported in Tables 1 and 2;
- For the calibration of instruments used in the determination of the concentration of analytes reported in Tables 1 and 2. When a value provided in this certificate is used to calibrate a measurement process, the uncertainty associated with that value should be appropriately propagated into the user's uncertainty calculation. Users can determine an approximation of the standard uncertainty by calculating one fourth of the width of the Expanded Uncertainty interval given in this certificate (Expanded Uncertainty intervals are provided in Tables 1 and 2).

MINIMUM SAMPLE SIZE

To relate analytical determinations to the values in this certificate, the minimum mass of sample used should match the typical mass that the laboratories used in the interlaboratory (round robin) certification program. This means that different minimum sample masses should be used depending on the operationally defined methodology as follows:

- Lithium borate fusion with X-ray fluorescence finish: $\geq 0.2\text{g}$;
- Loss on Ignition (LOI) at 1000°C : $\geq 1\text{g}$;
- C and S by infrared combustion furnace/CS analyser: $\geq 0.1\text{g}$;
- Cu and Co by 5% sulphuric acid leach with ICP or AAS finish: 0.5g ;
- Sodium peroxide fusion with ICP-OES and/or MS finish: $\geq 0.2\text{g}$;
- 4-acid digestion with ICP-OES and/or MS finish: $\geq 0.25\text{g}$;
- Aqua regia digestion with ICP-OES and/or MS finish: $\geq 0.5\text{g}$.

PERIOD OF VALIDITY & STORAGE INSTRUCTIONS

The certification of OREAS 556b remains valid, within the specified measurement uncertainties, until September 2033, provided the CRM is handled and stored in accordance with the instructions given below. This certification is nullified if the CRM is any way changed or contaminated.

Store in a clean and cool dry place away from direct sunlight.

Long-term stability will be monitored at appropriate intervals and purchasers notified if any changes are observed. The period of validity may well be indefinite and will be reassessed prior to expiry with the aim of extending the validity if possible.

Single-use sachets (e.g., 10g units)

Following analysis of the CRM subsample it is the manufacturers' expectation that any remaining material is discarded. The stability of the material after opening the sachet is not within the scope of proper use. However, if opened sachets are resealed after opening, then under ordinary* storage conditions the CRM will have a shelf-life beyond ten years.

**Ordinary storage conditions: means storage not in direct sunlight in a dry, clean, well ventilated area at temperatures between -5° and 50°C.*

INSTRUCTIONS FOR HANDLING & CORRECT USE

Pre-homogenisation of the CRM prior to subsampling and analysis is not necessary as there is no particle segregation under transport [12].

Fine powders pose a risk to eyes and lungs and therefore standard precautions including the use of safety glasses and dust masks are advised.

QC monitoring using multiples of the Standard Deviation (SD)

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program.

The majority of data generated in the round robin program was produced by a selection of world class laboratories. The SD's thus generated are more constrained than those that would be produced across a randomly selected group of laboratories. To produce more generally achievable SD's the 'pooled' SD's provided in this report include interlaboratory bias. This 'one size fits all' approach may require revision at the discretion of the QC manager concerned following careful scrutiny of QC control charts.

The performance gates shown in Table 6 are intended only to be used as a preliminary guide as to what a laboratory may be able to achieve. Over a period of time monitoring your own laboratory's data for this CRM, SD's should be calculated directly from your own laboratory's process. This will enable you to establish more specific performance gates that are fit for purpose for your application as well as the ability to monitor bias. If your long-term trend analysis shows an average value that is within the 95% expanded uncertainty then generally there is no cause for concern in regard to bias.

For use with the aqua regia digestion method

It is important to note that in the analytical industry there is no standardisation of the aqua regia digestion process. This method is a partial empirical digest and differences in recoveries for various analytes are commonplace. These are caused by variations in the digest conditions and can include the ratio of nitric to hydrochloric acids, acid strength, temperatures, leach times and secondary digestions. Recoveries for sulphide-hosted base metal sulphides approach total values, however, other analytes, in particular the lithophile elements, show greater sensitivity to method parameters. This can result in lack of consensus in an inter-laboratory certification program for these elements.

The approach applied here is to report certified values in those instances where reasonable agreement exists amongst a majority of participating laboratories. The results of specific laboratories may differ significantly from the certified values, but will, nonetheless, be valid

and reproducible in the context of the specifics of the aqua regia method in use. Users of this reference material should, therefore, be mindful of this limitation when applying the certified values in a quality control program.

LEGAL NOTICE

Ore Research & Exploration Pty Ltd has prepared and statistically evaluated the property values of this reference material to the best of its ability. The Purchaser by receipt hereof releases and indemnifies Ore Research & Exploration Pty Ltd from and against all liability and costs arising from the use of this material and information.

© 2024 COPYRIGHT Ore Research & Exploration Pty Ltd.
 Unauthorised copying, reproduction, storage or dissemination is prohibited.

DOCUMENT HISTORY

Revision No.	Date	Changes applied
0	7 th March, 2024	First publication.

CERTIFYING OFFICER



7th March, 2024

Craig Hamlyn (B.Sc. Hons - Geology), Technical Manager - ORE P/L

QMS CERTIFICATION

ORE Pty Ltd is accredited for compliance with ISO 17034:2016.



ORE Pty Ltd is ISO 9001:2015 certified by Lloyd's Register Quality Assurance Ltd for its quality management system including development, manufacturing, certification and supply of CRMs.



REFERENCES

- [1] Govett, G.J.S. (1983). Handbook of Exploration Geochemistry, Volume 2: Statistics and Data Analysis in Geochemical Prospecting (Variations of accuracy and precision).
- [2] ISO Guide 30:2015. Terms and definitions used in connection with reference materials.
- [3] ISO Guide 31:2015. Reference materials – Contents of certificates and labels.
- [4] ISO Guide 35:2017. Certification of reference materials - General and statistical principals.
- [5] ISO Guide 98-3:2008. Guide to the expression of uncertainty in measurement (GUM:1995).
- [6] ISO 16269:2014. Statistical interpretation of data – Part 6: Determination of statistical tolerance intervals.
- [7] ISO/TR 16476:2016, Reference Materials – Establishing and expressing metrological traceability of quantity values assigned to reference materials.
- [8] ISO 17025:2017, General requirements for the competence of testing and calibration laboratories.
- [9] ISO 17034:2016. General requirements for the competence of reference material producers.
- [10] Munsell Rock Color Book (2014). Rock-Color Chart Committee, Geological Society of America (GSA), Minnesota (USA).
- [11] OREAS-BUP-70-09-11: Statistical Analysis - OREAS Evaluation Method.
- [12] OREAS-TN-04-1498: Stability under transport; an experimental study of OREAS CRMs.
- [13] OREAS-TN-05-1674: Long-term storage stability; an experimental study of OREAS CRMs.
- [14] Thompson, A.; Taylor, B.N.; Guide for the Use of the International System of Units (SI); NIST Special Publication 811; U.S. Government Printing Office: Washington, DC (2008); available at: <https://physics.nist.gov/cuu/pdf/sp811.pdf> (accessed Jan 2024).
- [15] Van der Veen AMH and Pauwels, J. (2001). Uncertainty calculations in the certification of reference materials, Accred Qual Assur 6: 290-294.

APPENDIX

For Cu and Co by the two sulphuric acid leaches, specific methodologies were detailed for the participating laboratories to follow:

5% sulphuric acid leach

1. Weigh 0.500 ± 0.002 g of sample pulp into a clean 250 ml flask.
2. Add to the flask 0.5g of Sodium Sulphite (AR Grade).
3. Add 50 ml of approximately 55 g/l Sulphuric acid solution (prepared from a 98% pure concentrated sulphuric acid).
4. Put the cap on the flask and start automatic shaking. Leave the sample on continuous shaking to leach for four (4) hours.
5. Remove the cap and add 25 ml of hydrochloric acid.
6. Dilute to a final volume of 250 ml with distilled/deionised water up to the mark and mix again by inverting at least 10 times. Allow the solution to settle for 30 minutes.
7. The solution is now ready to be analysed by ICP or AAS.